



Medtronic

User Guide

CareLink[®] Pro

THErapy MANAGEMENT SOFTWARE FOR DIABETES



Medtronic



Medtronic MiniMed
18000 Devonshire Street
Northridge, CA 91325
USA
800 646 4633
818 576 5555

EC REP

Medtronic B.V.
Earl Bakkenstraat 10
6422 PJ Heerlen
The Netherlands



6025179-028_b
REF MMT-7335

© 2011 Medtronic MiniMed, Inc. All rights reserved.

MiniMed™, Paradigm™, Paradigm Link™, Guardian™, Veo™, REAL-Time™, CareLink™, Dual Wave™, Square Wave™, Easy Bolus™, SmartGuard™, and Bolus Wizard™ are trademarks of Medtronic MiniMed, Inc.

BD Logic® is a registered trademark of Becton, Dickinson and Company.

CONTOUR™, GLUCOFACTS™ DELUXE, GLUCOMETER™, DEX™, ELITE™, and BREEZE™ are trademarks of Bayer.

OneTouch®, OneTouch® Profile®, OneTouch® Ultra®, OneTouch® UltraSmart®, OneTouch® Basic®, OneTouch® FastTake®, OneTouch® SureStep®, OneTouch® UltraMini®, OneTouch® Ultra® 2, and OneTouch® UltraEasy® are trademarks of LifeScan, Inc.

Optium Xceed™, Precision Xceed™, Precision Xtra®, FreeStyle®, Therasense FreeStyle®, FreeStyle® Flash®, FreeStyle® Mini®, FreeStyle® Freedom®, FreeStyle® Lite®, FreeStyle® Freedom Lite®, and FreeStyle Papillon™ mini are trademarks of Abbott Laboratories, Inc.

ACCU-CHEK® Active, ACCU-CHEK® Aviva, ACCU-CHEK® Compact, and ACCU-CHEK® Compact Plus are registered trademarks of a member of the Roche Group.

Java™ is a trademark of Sun Microsystems, Inc.

Microsoft®, Windows®, and Excel® are registered trademarks of Microsoft Corporation.

Adobe® and Acrobat® Reader® are registered trademarks of Adobe Systems, Incorporated.

Contacts:**Africa:**

Medtronic Africa (Pty) Ltd.
Tel: +27 (0) 11 677 4800

Australia:

Medtronic Australasia Pty. Ltd.
Tel: 1800 668 670 (product orders)
Tel: 1800 777 808 (customer help)

Azerbaijan:

Albatros Health Care
Tel: +994 12 498 9537

Bangladesh

Sonargaon Healthcare Pvt Ltd.
Mobile: (+91)-9903995417
or (+880)-1714217131

Belarus:

Badgin Ltd
Tel: +375 (172) 665128

België/Belgique:

N.V. Medtronic Belgium S.A.
Tel: 0800-90805

Bosnia and Herzegovina

Intermedical
Tel: +387 33 202 183
Fax: +387 33 202 183

Brasil:

Medtronic Comercial Ltda.
Tel: +(11) 3707-3707

Bulgaria

Interagro-90 Ltd
Tel: +359 888 636 033

Canada:

Medtronic of Canada Ltd.
Tel: 1-800-284-4416 (toll free/sans-frais)

China:

Medtronic (Shanghai) Ltd.
24 Hour Help (Cell): +86 400-820-1981
24 Hour Help (Landline): +86 800-820-1981

Croatia

Oktal Pharma
Tel: +385 1 659 57 77
Fax: +385 1 659 57 01

Croatia

Medtronic B.V.
Tel: +385 1 488 11 20
Fax: +385 1 484 40 60

Danmark:

Medtronic Danmark A/S
Tel: +45 32 48 18 00

Deutschland:

Medtronic GmbH
Geschäftsbereich Diabetes
Telefon: +49 2159 8149-370
Telefax: +49 2159 8149-110
24-Std-Hotline: 0800 6464633

Eire:

Accu-Science LTD.
Tel: +353 45 433000

España:

Medtronic Ibérica S.A.
Tel: +34 91 625 05 42
Fax: +34 91 625 03 90
24 horas: +34 901 120 335

Europe:

Medtronic Europe S.A. Europe, Middle East and Africa
Headquarters
Tel: +41 (0) 21-802-7000

France:

Medtronic France S.A.S.
Tel: +33 (0) 1 55 38 17 00

Hellas:

Medtronic Hellas S.A.
Tel: +30 210677-9099

Hong Kong:

Medtronic International Ltd.
Tel: +852 2919-1300
To order supplies: +852 2919-1322
24-hour helpline: +852 2919-6441

India:

India Medtronic Pvt. Ltd
Tel: (+91)-80-22112245 / 32972359
Mobile: (+91)-9611633007

Indonesia:

Medtronic International Ltd.
Tel: +65 6436 5090
or +65 6436 5000

Israel:

Agentek
Tel: +972 3649 3111

Italia:

Medtronic Italia S.p.A.
Tel: +39 02 24137 261
Fax: +39 02 24138 210
Servizio assistenza tecnica:
N° verde 24h: 800 20 90 20

Japan:

Medtronic Japan Co. Ltd.
Tel: +81-3-6430-2019
24 Hr. Support Line: 0120-56-32-56

Kazakhstan:

Medtronic Kazakhstan B.V.
Tel: +77273110580

Latin America:

Medtronic, Inc.
Tel: 1(305) 500-9328
Fax: 1(786) 709-4244

Latvija:

Ravemma Ltd.
Tel: +371 7273780

Macedonia:

Kemofarm
Tel: +389 2 260 36 03
Fax: +389 2 260 36 49

Magyarország:

Medtronic Hungária Kft.
Tel: +36 1 889 0688

Malaysia:

Medtronic International Ltd.
Tel: +603 7946 9000

Middle East and North Africa:

Regional Office
Tel: +961-1-370 670

Montenegro:

Glosarij
Tel: +382 20 642 495
Fax: +382 20 642 540

Nederland, Luxembourg:

Medtronic B.V.
Tel: +31 (0) 45-566-8291
Gratis: 0800-3422338

New Zealand:

Medica Pacifica
Phone: 64 9 414 0318
Free Phone: 0800 106 100

Norge:

Medtronic Norge A/S
Tel: +47 67 10 32 00
Fax: +47 67 10 32 10

РОССИЯ:

Medtronic B. V.
Tel: +7 495 580 73 77
24h: 8-800-200-76-36

Philippines:

Medtronic International Ltd.
Tel: +65 6436 5090
or +65 6436 5000

Polska:

Medtronic Poland Sp. Z.o.o.
Tel: +48 22 465 6934

Portugal:

Medtronic Portugal Lda
Tel: +351 21 7245100
Fax: +351 21 7245199

Puerto Rico:

Medtronic Puerto Rico
Tel: 787-753-5270

Republic of Korea:

Medtronic Korea, Co., Ltd.
Tel: +82.2.3404.3600

Romania:

Trustmed SRL
Tel: +40 (0) 21 220 6477

Schweiz:

Medtronic (Schweiz) AG
Tel: +41 (0)31 868 0160
24-Stunden-Hotline: 0800 633333
Fax Allgemein: +41 (0)318680199

Serbia

Epsilon
Tel: +381 11 311 5554
Fax: +381 11 311 5554

Singapore:

Medtronic International Ltd.
Tel: +65 6436 5090
or +65 6436 5000

Slovenija:

Zaloker & Zaloker d.o.o.
Tel: +386 1 542 51 11
24-h pomoč: 386 51 316 560

Slovenská republika:

Medtronic Slovakia o.z.
Tel: +421 26820 6986
Fax: +421 268 206 999

Sri Lanka

Swiss Biogenics Ltd.
Mobile: (+91)-9003077499
or (+94)-777256760

Suomi:

Medtronic Finland Oy
Tel: +358 20 7281 200
Help line: +358 400 100 313

Sverige:

Medtronic AB
Tel: +46 8 568 585 20
Fax: +46 8 568 585 11

Taiwan:

Medtronic-Taiwan Ltd.
Tel: +886.2.2183.6068
Toll Free: +886.0800.005.285

Thailand:

Medtronic (Thailand) Ltd.
Tel: +662 232 7400

Turkiye:

Medtronic Medikal Teknoloji
Ticaret Ltd. Sirketi.
Tel: +90 216 4694330

USA:

Medtronic Diabetes Global Headquarters
Tel: +1-800-646-4633
24 Hour HelpLine: +1-800-826-2099
To order supplies: +1-800-843-6687

Ukraine:

Med EK Service Ltd.
Tel: +380445457705

United Kingdom:

Medtronic Ltd.
Tel: +44 1923-205167

Österreich:

Medtronic Österreich GmbH
Tel: +43 (0) 1 240 44-0
24 – Stunden – Hotline: 0820 820 190

Česká republika:

Medtronic Czechia s.r.o.
Tel: +420 233 059 401
Non-stop help line:
+420 233 059 059

Contents

Chapter 1	1	Introduction
	1	Features
	2	Security
	2	Assistance
	2	Supported devices
	4	Ordering
	4	How to use this guide
	5	User safety
Chapter 2	7	Getting started
	7	Before you begin
	7	Primary system tasks
	8	Navigating the system
	8	Opening CareLink Pro
	8	Workspaces
	8	Toolbar
	9	Patient tabs
	9	The Guide Me feature
	9	Turning Guide Me on and off
	10	Opening patient records
	10	Closing patient records
	11	Setting system preferences
	11	General preferences
	12	Patient profile preferences
	13	Choosing data fields
	13	Adding a custom field
	13	Changing the order of data fields
	14	Finalizing patient profile preferences
	14	Patient Lookup preferences
	14	Choosing data to display
	14	Changing the column order
	15	Finalizing patient lookup preferences
	15	Report Generation preferences

	15	Choosing data to display
	17	Changing the column order
	17	Finalizing report generation preferences
Chapter 3	18	Profile workspace
	18	Before you begin
	19	Adding new profiles
	19	Editing patient profiles
	19	Deleting patient data from the system
	20	Linking to CareLink Personal
Chapter 4	23	Hardware setup
	24	Connecting devices
Chapter 5	26	Devices workspace
	26	Before you begin
	27	Adding a device
	27	Adding a Medtronic pump or Guardian monitor
	30	Adding a meter
	32	Making a device active or inactive
	33	Reading device data
Chapter 6	35	Reports workspace
	35	Before you begin
	36	Creating reports
	36	Opening the Reports workspace
	36	Selecting the reporting period
	36	Data calendar
	37	Selecting source data to include
	37	Checking for device data
	38	Getting additional device data
	39	Verifying report settings
	40	Selecting report types and inclusion dates
	41	Generating reports
	41	About reports
	41	Dashboard and Episode Summary
	42	Therapy Management Dashboard
	42	Episode Summary
	42	Adherence Report
	42	Sensor and Meter Overview Report
	43	Logbook Report
	43	Device Settings Snapshot
	43	Daily Detail Report
	43	Exporting data
Chapter 7	45	System administration
	45	Applying software updates

	45	Backing up and restoring the database
	45	Backing up the database
	46	Restoring the database
	46	When the system is unavailable
Chapter 8	47	Troubleshooting
	47	Not connected to the database
	47	Forgot the clinic password for CareLink Pro
	47	Device read errors
	49	Report creation errors
	50	Backup and restore errors
	50	Uninstalling the software
Chapter 9	51	Icon table
Appendix A	52	CSV data
	52	Column data definitions
	54	More about CSV files exported by CareLink Pro
	54	If data is not displaying as expected
Glossary	55	
Index	59	

Introduction

Thank you for choosing Medtronic Diabetes as your partner in helping you and your patients better manage diabetes therapy. We believe you will benefit from CareLink™ Pro software's leading edge technology and simple, menu-driven user interface.

CareLink Pro allows you to acquire, store, and report patient treatment and diagnostic data. You can also use it to access pump, meter, and sensor-based glucose data your patients have uploaded to CareLink™ Personal, a web-based therapy management system that works with CareLink Pro.

Features

CareLink Pro is a diabetes therapy management software for a personal computer (PC).

- Patient records can be created to store data gathered from a patient's device as well as therapy data from his or her CareLink Personal account.
- Data from insulin pumps, monitors, and blood glucose meters can be sent to the system, stored, and then used to generate reports.
- As an option, CareLink Pro interfaces with the CareLink Personal system, allowing access to device data patients have stored there. This is ideal for creating current reports between office visits, and may make the need to read device data during office visits unnecessary.
- Different treatment reports can be created from device data stored in the patient's record. Reports facilitate answers to therapy concerns, such as patient adherence, patterns, and exceptions.
- The Guide Me feature helps users who are new to CareLink Pro. It gives hints and tips about the tasks they are performing.
- An integrated help system is available throughout the software to provide information on specific areas of interest.

Security

- CareLink Pro can be password protected.
- Transmission of patient data from CareLink Personal is encrypted using industry-standard Secure Sockets Layer (SSL) technology.

Assistance

If you need further help with this system, contact your local country representative. Access the following web site for international contact information:

<http://www.medtronicdiabetes.com/contact/international-locations>

Supported devices

CareLink Pro gets data from the following devices.

NOTE: Some devices supported by this software may not be available in all countries where this software is approved for use.

MiniMed insulin pumps/Guardian glucose monitors	
MiniMed™ pumps	MiniMed 640G (MMT-1511, MMT-1512, MMT-1711, MMT-1712), part of the MiniMed 600 series pumps MiniMed Paradigm™ series pumps: <ul style="list-style-type: none"> • MiniMed Paradigm Veo (MMT-554, MMT-754) • MiniMed Paradigm (MMT-522, MMT-722, MMT-522K, MMT-722K, MMT-515, MMT-715, MMT-512, MMT-712, MMT-511) MiniMed 508 pump (MMT-508)
Guardian™ REAL-Time™ monitors	Guardian REAL-Time Continuous Glucose Monitoring System (CSS7100, CSS7100K)

Manufacturer	Blood glucose meters
Link meters	<ul style="list-style-type: none"> • Bayer CONTOUR™ PLUS LINK 2.4 • Bayer CONTOUR™ NEXT LINK 2.4 • Bayer CONTOUR™ NEXT LINK • Bayer CONTOUR™ LINK • BD Paradigm Link™ Blood Glucose Monitor
Bayer	<ul style="list-style-type: none"> • CONTOUR™ XT • CONTOUR™ USB • BREEZE™ • BREEZE™ 2 • CONTOUR™

Manufacturer	Blood glucose meters
LifeScan	<ul style="list-style-type: none"> • OneTouch® UltraSmart® • OneTouch® Profile® • OneTouch® Ultra® • OneTouch® Basic® • OneTouch® FastTake® • OneTouch® SureStep® • OneTouch® Ultra® 2 • OneTouch® UltraMini® • OneTouch® UltraEasy®
BD	<ul style="list-style-type: none"> • Logic®
Bayer DEX™ family, including these compatible meters	<ul style="list-style-type: none"> • DEX™ • DEX™ 2 • DEXTER-Z™ II • Glucometer™ DEXTER-Z™ • ESPRIT™ 2 • Glucometer™ ESPRIT™ • Glucometer™ ESPRIT™ 2
Bayer ELITE™ family, including these compatible meters	<ul style="list-style-type: none"> • ELITE™ • Glucometer™ ELITE™ XL
Abbott	<ul style="list-style-type: none"> • FreeStyle® • FreeStyle® Lite® • FreeStyle® Freedom® • FreeStyle® Freedom Lite® • Precision Xtra® • TheraSense FreeStyle® • FreeStyle® Flash® • FreeStyle® Papillon™ mini • FreeStyle® Mini® • Optium Xceed™ • Precision Xceed™
Roche	<ul style="list-style-type: none"> • Accu-Chek® Aviva • Accu-Chek® CompactPlus • Accu-Chek® Compact • Accu-Chek® Active

Communication devices	
Bayer CONTOUR™ PLUS LINK 2.4 Bayer CONTOUR™ NEXT LINK 2.4	For uploading the MiniMed 600 series insulin pumps.
Bayer CONTOUR™ NEXT LINK	For uploading the MiniMed Paradigm series insulin pumps and Guardian REAL-Time Monitor.
Medtronic MiniMed Com-Station (MMT-7301)	For uploading the MiniMed 508 pump. See the Com-Station User Guide for details about the required hardware.
Medtronic MiniMed CareLink USB (MMT-7306, black)	For uploading the MiniMed 600 series insulin pumps.
Medtronic MiniMed CareLink USB (MMT-7305, white)	For uploading the MiniMed Paradigm series insulin pumps and Guardian REAL-Time Monitor.

Communication devices	
Paradigm Link™ Blood Glucose Monitor	For uploading a MiniMed Paradigm Pump or Guardian REAL-Time Monitor. See the Paradigm Link Blood Glucose Monitor User Guide for details about the required hardware.
Medtronic MiniMed ComLink (MMT-7304)	For uploading the MiniMed Paradigm series insulin pumps and Guardian REAL-Time Monitor. See the ComLink User Guide for details about the required hardware.
Data communications cable	<p>For uploading data from third-party blood glucose meters. Each meter manufacturer supplies a data communications cable.</p> <p>Note: If a meter manufacturer provides a USB cable instead of a serial cable for uploading data, you must install the software driver provided by that manufacturer.</p> <p>Also, check with the meter manufacturer to ensure that the USB driver is compatible with your operating system. Some USB drivers may not be available for 64-bit operating systems.</p>

Equivalent devices

When you add a device to the system, you select its make and model from a list. If a device make and model is not on the list, refer to the following table to find an equivalent one to use.

If your patient uses one of these devices	Select this device
<ul style="list-style-type: none"> • Bayer DEX™ 2 • Bayer DEXTER-Z™ II • Bayer Glucometer™ DEXTER-Z™ • Bayer ESPRIT™ 2 • Bayer Glucometer™ ESPRIT™ • Bayer Glucometer™ ESPRIT™ 2 	Bayer DEX™
Bayer Glucometer™ ELITE™ XL	Bayer ELITE™
Abbott Precision Xceed™	Abbott Optium Xceed™

Ordering

To order Medtronic Diabetes products, contact your local country representative. Access the following URL for international contact information:

<http://www.medtronicdiabetes.com/contact/international-locations>

NOTE: Meters can be ordered from their respective companies.

How to use this guide

NOTE: This user guide shows samples of the software screens. The screens of the actual software may be slightly different.

Refer to the Glossary for definitions of terms and functions. The conventions used in this guide are defined in the following table.

Term/style	Meaning
Click	Press the left mouse button over an object on the screen to select it.
Double-click	Press the left mouse button twice over an object on the screen to open it.
Right-click	Press the right mouse button over an object on the screen to display another window or menu.
Bold text	Used for a button, screen name, field name, or menu option. For example: Patient > New Patient
NOTE:	Provides additional information for a procedure or step.
CAUTION:	Alerts you of a potential hazard which, if not avoided, may result in minor or moderate damage to the software program or equipment.
WARNING:	Notifies you of a potential hazard which, if not avoided, could result in death or a serious injury. It may also describe potential serious adverse reactions and safety hazards.

User safety

Indications for use

The CareLink Pro system is intended for use as a tool to help manage diabetes. The purpose of this system is to take information transmitted from insulin pumps, glucose meters, and continuous glucose monitoring systems, and turn it into CareLink Pro reports. The reports provide information that can be used to identify trends and track daily activities—such as carbohydrates consumed, meal times, insulin delivery, and glucose readings.

Warnings

- This system is intended to be used by a healthcare professional familiar with the management of diabetes.
- System results are not intended to produce medical advice and should not be relied upon for such purpose.
- This product should only be used with the supported devices listed in this document. (See [Supported devices on page 2.](#))
- Patients should be advised to monitor their blood glucose levels at least 4–6 times a day.
- Patients should be advised not to make any changes to their treatment without consulting their healthcare professional.
- Patients should be advised to make treatment decisions based on healthcare professional guidelines and meter BG results, not sensor glucose results.

Contraindications

This software should not be used with devices that are not listed in [Supported devices on page 2](#). Nor should this product be used for the treatment of medical conditions other than diabetes.

Before opening this software, close any of the following software that is currently running on your computer:

- CGMS™ System Solutions™ Software (MMT-7310)
- Solutions™ Pumps & Meters Software (MMT-7311)
- Guardian™ Solutions Software (MMT-7315)
- ParadigmPAL™ (MMT-7330)
- CareLink™ Personal Software (MMT-7333)
- Solutions Software for CGMS iPro (MMT-7319)

Getting started

The following information will guide you through starting the CareLink Pro software, opening and closing patient records, and setting preferences that apply to all patients in the system.

Before you begin

If this is the first time you are using CareLink Pro, you should be sure to set the General preferences (see [General preferences on page 11](#)). These preferences determine how certain items display in the software and in reports, and how you want the system to communicate with the Internet.

Preferences can be set at any time. You may want to wait until you are familiar with the CareLink Pro software to set the other preferences.

Primary system tasks

The following table outlines the main tasks you will need to perform when first setting up and using CareLink Pro. It also tells you which part of this user guide discusses each task.

Step	Location
Familiarize yourself with the CareLink Pro user interface.	Navigating the system on page 8
Define the global system options your clinic will use.	Setting system preferences on page 11
Create profiles for each of your patients.	Adding new profiles on page 19
Link to your patients' CareLink Personal accounts.	Linking to CareLink Personal on page 20
Add your patient's pump and meters to his or her profile.	Adding a device on page 27
Read data from your patient's pump and meters.	Reading device data on page 33
Set up and generate reports for each of your patients.	Creating reports on page 36
Regularly back up the CareLink Pro database.	Backing up the database on page 45
Update the CareLink Pro software.	Applying software updates on page 45

Navigating the system

Before working with the CareLink Pro software, you should get acquainted with the user interface. The user interface includes menus, a toolbar, a navigation bar, workspaces, and a Guide Me window.

Opening CareLink Pro

- 1 Double-click the CareLink Pro icon  on your computer desktop, or select **Medtronic CareLink Pro** from the Programs list on your Windows® Start menu. If you are using Windows 8, click the **Medtronic CareLink Pro** tile on the Start screen.

If your clinic requires you to enter a password, the login screen is displayed.

- a. Type your password into the **Password** field.

NOTE: Requiring a password is an optional feature that is set during the installation process.

- b. Click **LOGIN**.

The startup screen is displayed.

- 2 To start a new patient record, click **New Patient**. To open a patient record from a list of patients in the system, click **Open Patient**.

Workspaces

If you have a patient's record open, you can click one of the buttons on the navigation bar to display the corresponding workspace. Use these workspaces to enter or select information to perform CareLink Pro tasks for that patient.

	Profile: Allows you to maintain such patient information stored as name and date of birth. This workspace also allows you to link to a patient's CareLink Personal account.
	Devices: Allows you to store information required to read a patient's devices.
	Reports: Allows you to select parameters and choose reports to be generated for the patient.

Until a profile is added and saved for a patient, only the Profile workspace is accessible for that patient. Until devices are added for a patient, only the Profile and Devices workspaces are accessible for that patient.

Toolbar

The CareLink Pro toolbar provides quick access to frequently used features. The toolbar contains the following buttons.

Button	Name	Functionality
	Add Patient	Opens a Profile workspace so you can add a new patient record to the system.
	Open Patient	Opens the Patient Lookup table where you can choose an existing patient's record to view.
	Guide Me	Displays or hides the Guide Me window. Click for basic context-aware hints.

Patient tabs

After you open a patient record, a tab is displayed along the toolbar with the patient's name on it. When a tab is active, it means that patient record and workspace are active, and you can perform CareLink Pro tasks for the patient.



To make a patient record active so that you can work with it, click on the tab for that patient. To close a patient record, click the **Close** button  on the tab.

The Guide Me feature

A Guide Me feature is provided throughout CareLink Pro. It opens a window with context-aware hints and tips for actions you might take from the part of system that is active. Guide Me windows might also include **>>learn more** links. When clicked, these links take you to the relevant section in the online help for more details. The Guide Me feature is enabled by default. However, you can turn it off at any time.



Turning Guide Me on and off

To turn Guide Me on or off, do one of the following:


- Click the **Guide Me** button. 

- Select **Help > Guide Me**.

Opening patient records

As many as six patient records can be open at one time. If you have not yet created any patient profiles, see [Adding new profiles on page 19](#).

- 1 Select **File > Open Patient**, or click the **Open Patient** button.  A patient list similar to the following is displayed.

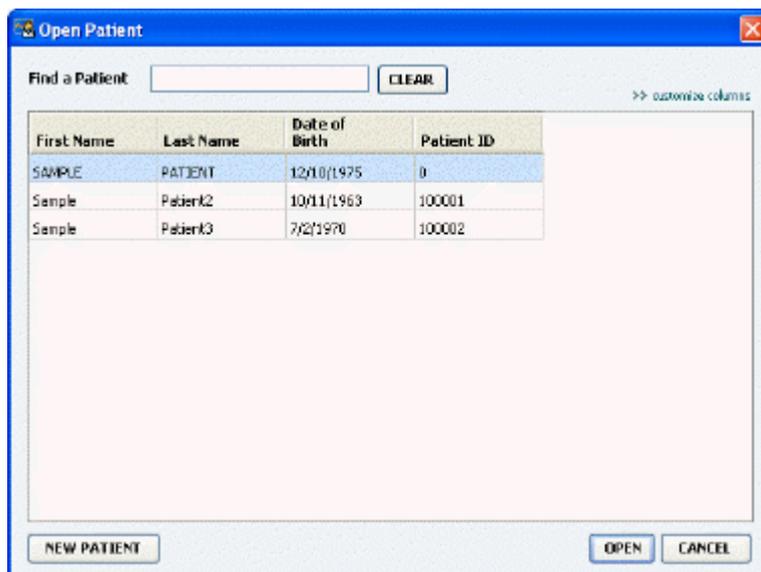

NOTE: If you receive a message that you have too many patient records open, click **OK**, close a record, and continue.

- 2 Locate the patient's listing by typing some or all of his or her name in the **Find a Patient** field. When the patient's listing is highlighted, click **OPEN**, double-click the listing, or press ENTER. You can also navigate the list by using the up and down arrows on your keyboard. The patient's **Devices** (if devices have not yet been added) or **Reports** workspace is displayed.
- 3 To see the patient's **Profile** workspace, click the **Profile** button  on the navigation bar.

Closing patient records

- 1 Make sure the patient record you want to close is active (the tab is highlighted).
- 2 Do one of the following:
 - a. Select **File > Close Patient**.
 - b. Click the **Close** button  on the patient tab.
 - c. Press Ctrl+F4.

Setting system preferences

These preferences apply to all patients in the system. For preferences that affect only individual patients, see [Verifying report settings on page 39](#).


Preferences are displayed in the following groups:

- General
 - Glucose units
 - Carbohydrate units
 - Communications
 - Troubleshooting
- Patient Profile
 - Select and arrange data fields on patient profiles.
- Patient Lookup
 - Modify and change the order of fields displayed when you choose Open Patient to view a list of patients.
- Report Generation
 - Choose the data fields you want to display when selecting Daily Detail report input from the Data table.

General preferences

Use the General tab to define how the software displays certain types of information and to establish your external communication preferences.

- 1 If it is not active already, click the **General** tab.
- 2 Select **Tools > Options**. The following window is displayed.

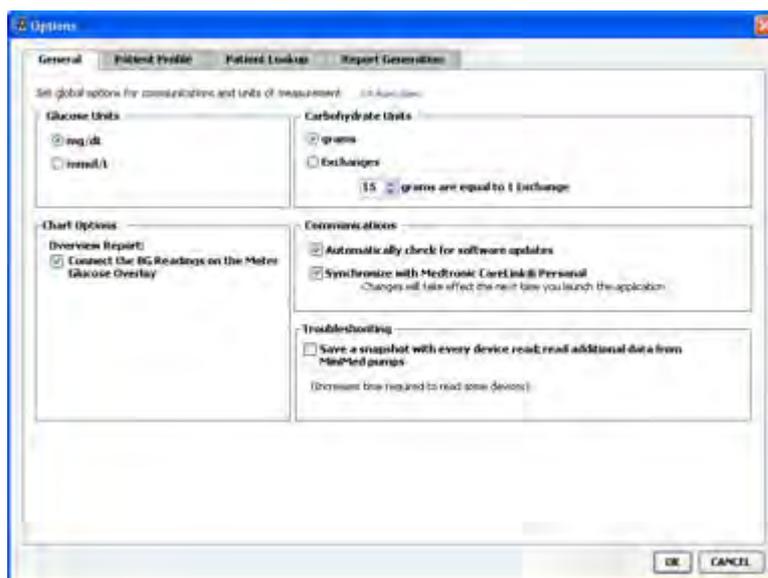

- 3 Click to select the option button for the value you want:

- **Glucose Units:** mmol/L or mg/dL
 - **Carbohydrate Units:** grams or Exchanges
 - a. If you selected **Exchanges** for **Carbohydrate Units**, type the appropriate number in the **grams are equal to 1 Exchange** field.
- 4 Click to select or clear the check box in the Chart Options > Overview Report section. If the check box is selected, the application will connect the BG readings on the Meter Glucose Overlay chart with lines. (This is a chart that appears in the Sensor and Meter Overview Report.)
 - 5 For the following Communications preferences, click to select the check box (enable) or to clear the check box (disable):

NOTE: Make sure you follow the guidelines of your clinic or IT department when setting communication preferences.


- **Automatically check for software updates:** If selected, a notification will be sent to each system running CareLink Pro whenever a software update is available. The active user will then have the opportunity to download and install the updates. To prevent this from occurring and institute a controlled distribution of software updates, you can clear this check box.
 - **Synchronize with Medtronic CareLink Personal:** If you want the system to automatically synchronize your patients' CareLink Personal data each time you open their profile, select this check box. If you clear this check box, you will have to manually synchronize the CareLink Personal data for each patient.
- 6 Click to select or clear the check box in the **Troubleshooting** section. If the check box is selected, the application will save a record of device reads for troubleshooting purposes.
 - 7 Click **OK** to save the General preferences.

Patient profile preferences

This is a global setting that defines the content of your profiles. You can customize fields in the Profiles workspace to include information that is most important to your clinic. You can add or remove fields, create your own custom fields, and determine the order in which the fields will appear in the window.

- 1 Select **Tools > Options**.

- 2 Click the **Patient Profile** tab. The following window is displayed.

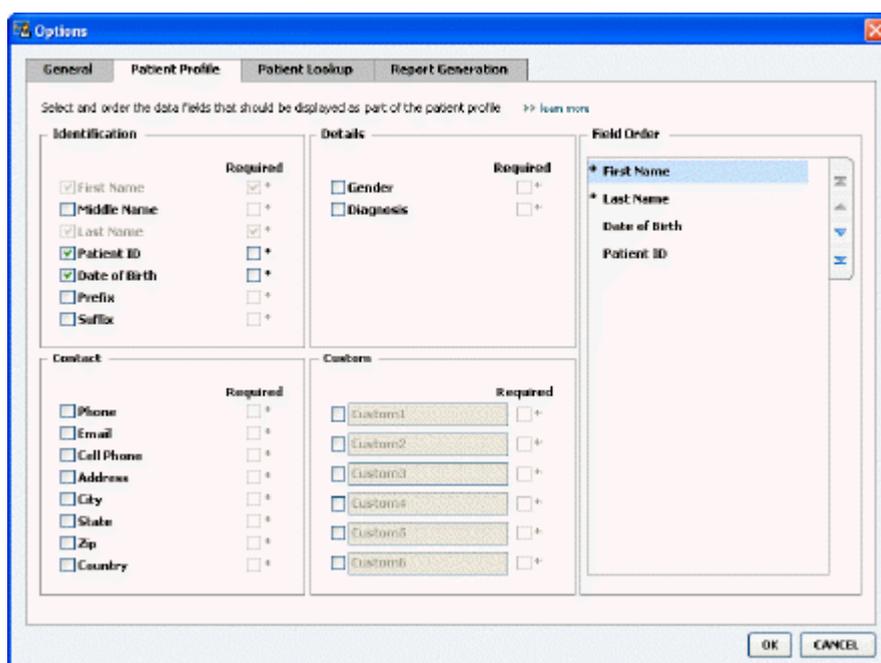

NOTE: Use the check boxes to choose the fields you want on the profile. Use the up and down arrows to put the fields in order.

Choosing data fields

- 1 Use the check boxes to add the fields you want.

NOTE: First and Last Name cannot be removed.

- 2 To remove a field from the profile, clear its check box.
- 3 To make a field required, select the check box in the **Required** column. Any field that is required must be filled in before a profile can be created.

Adding a custom field

- 1 Select the check box to the left of an empty custom field.
- 2 Enter text to name the field (for example, Emergency Contact). This is the field name that will display on the patient profile.
- 3 To make the field required, select the check box in the **Required** column.

NOTE: To remove a custom field from the profile, clear the check box next to the field(s) you want to remove.

Changing the order of data fields

Select the field you want to move, and click the up or down arrow  to move it. (The arrows at the top and bottom move a field all the way to the top or bottom of the list.)

Finalizing patient profile preferences


When the Field Order list has all the fields you want in the correct order, click **OK**.

Patient profiles now have the fields and field order you just selected.

Patient Lookup preferences

The Patient Lookup table is used to search for and open a patient record. The table includes every patient in your database and provides identifying information from the patient's profile. You have the option of customizing what information is displayed in this table and the order in which the columns appear. To customize the Patient Lookup table, complete the following steps:

- 1 Select **Tools > Options**.
- 2 Click the **Patient Lookup** tab. The following window is displayed.

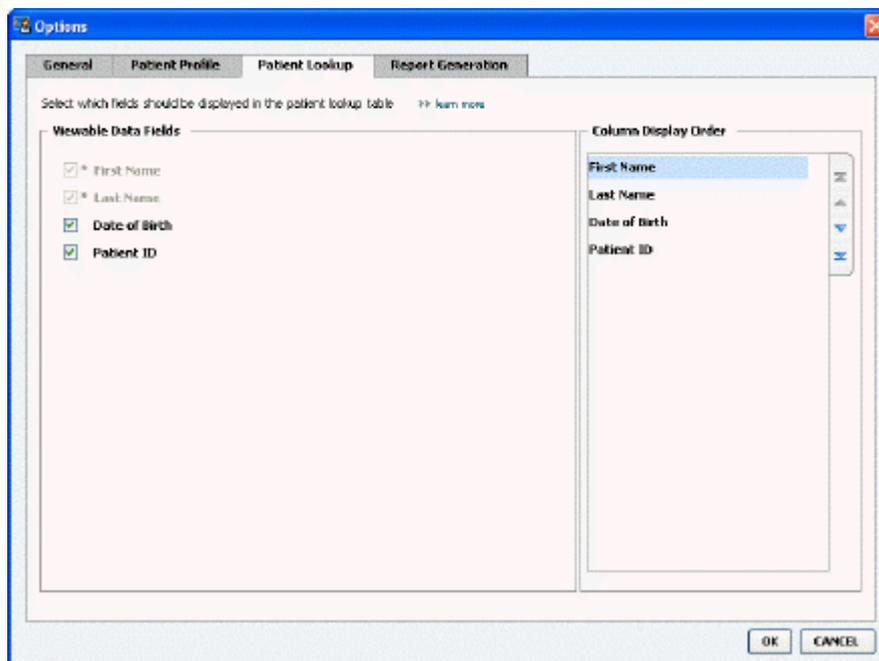

NOTE: Use the check boxes to choose the data you want on the Patient Lookup table. Use the up and down arrows to put the columns in order.

Choosing data to display

Use the check boxes to select the type of data you want to display or to clear data you do not want to display on the Patient Lookup table.

Changing the column order

To change the order of columns on the Patient Lookup table, select the column to move, and click the up or down arrows.  (The arrows at the top and bottom move a data column all the way to the top or bottom of the list.)

The data column at the top of the Column Display Order list will display in the first column of the Patient Lookup table. The data column at the bottom will be displayed in the last column of the table.

Finalizing patient lookup preferences

When the Column Display Order list has all the data you want in the correct order, click **OK**. The Patient Lookup table will now have the data and column order you just selected.


Report Generation preferences

The Data Table appears in the Select and Generate Reports window. This table is used during reporting. It contains daily information derived from your patient's devices and, if applicable, his or her CareLink Personal software account. The data provided in this table helps you determine which days require a Daily Detail report. It also helps you decide which of the other reports you should run.

Your clinic can customize the data that displays in this table, including the order in which it's presented, to reflect what is most relevant to your practice.

NOTE: To see how these preferences apply to the Data Table during report creation, see *Selecting report types and inclusion dates on page 40*.

- 1 Select **Tools > Options**.
- 2 Click the **Report Generation** tab. The following window is displayed.

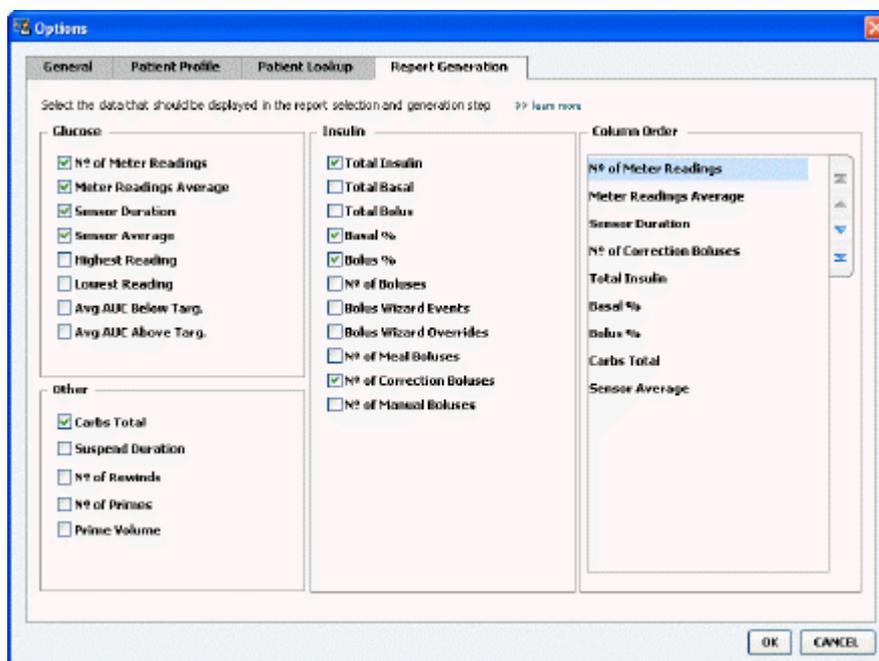

Choosing data to display

Use the check boxes to select the type of data you want to display or clear data you do not want to display on the Data Table.

The following information is available for inclusion in the Data Table.

Column Name	Definition
Nº of Meter Readings	The amount of readings for the specified date that were recorded by the included devices.
Meter Readings Average	The average of the glucose readings recorded by the included devices.
Sensor Duration	The amount of time within the specified date for which sensor data was recorded. Values are -- (none), 0:05 - 24:00.
Sensor Average	The average of sensor readings recorded in the specified date.
Highest Reading	The highest glucose reading (derived from a sensor or meter) for the date.
Lowest Reading	The lowest glucose reading (derived from a sensor or meter) for the date.
Avg AUC Below Target	Avg Area Under the Curve below the patient's target range.
Avg AUC Above Target	Avg Area Under the Curve above the patient's target range.
Total Carbs	The sum of all carbohydrate amounts (rounded to the nearest gram or the nearest 0.1 exchange, depending on the unit of measure used) reported during the day through Bolus Wizard™ events or carbohydrate markers on the pump or Guardian monitor.
Suspend Duration	The amount of time the pump was suspended on the specified date. Values are -- (no data), 0:01 - 24:00.
Nº of Rewinds	The number of rewind events for the specified date.
Nº of Primes (or Fills)	The number of prime events (or fill events) recorded for the specified date.
Prime (or Fill) Volume (U)	The total volume of insulin used for prime events (or fill events) on the specified date.
Total Insulin (U)	The total volume of insulin given during the specified date, as recorded by the pump.
Total Basal (U)	The total volume of basal insulin given during the specified date (the total insulin given, less the sum of all boluses given).
Total Bolus (U)	The total volume of insulin given in boluses during the specified date, as recorded by the pump.
Basal %	Shows the ratio (in whole % values) of basal insulin to total insulin.
Bolus %	Shows the ratio (in whole % values) of bolus insulin to total insulin.
Nº of Boluses	The number of bolus events recorded for the specified date.
Bolus Wizard Events	The total number of Bolus Wizard events recorded on the specified date.
Bolus Wizard Overrides	The number of Bolus Wizard events where the amount of insulin delivered is different than the amount recommended.
Nº of Meal Boluses	The number of Bolus Wizard events with carbohydrate amounts greater than zero that were recorded on the specified date.

Column Name	Definition
Nº of Correction Boluses	The number of Bolus Wizard events with correction amounts greater than zero that were recorded on the specified date.
Nº of Manual Boluses	The number of bolus events recorded during the date, which were not Bolus Wizard events.

Changing the column order

To change the order of columns on the Data Table, select the column to move, and click the up or down arrow.  (The top and bottom arrows move a data column all the way to the top or bottom of the list.)

NOTE: Items at the top of the Column Order list will display in the first column of the Data Table. Items at the bottom will display in the last column of the Data Table.


Finalizing report generation preferences

When the Column Order list has all the data you want in the correct order, click **OK**.

The Data Table will now have the data and column order you just selected.

Profile workspace

A profile is similar to the cover page of a medical chart. It stores patient data such as name and date of birth. A profile is required before device data can be gathered and used for therapy reports.

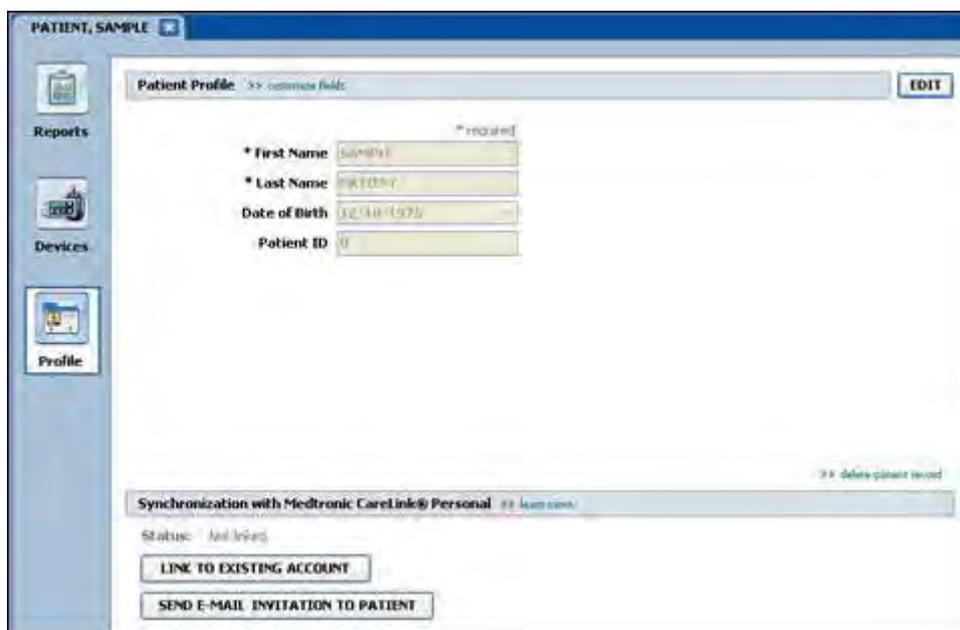

The screenshot shows the 'Patient Profile' workspace for a patient named 'SAMPLE'. The interface includes a sidebar with navigation options: Reports, Devices, and Profile. The main content area displays the following fields:

- * First Name: SAMPLE
- * Last Name: WOODS
- Date of Birth: 12/10/1975
- Patient ID: [Empty field]

At the bottom of the workspace, there is a section for 'Synchronization with Medtronic CareLink® Personal'. The status is 'Not linked', and there are two buttons: 'LINK TO EXISTING ACCOUNT' and 'SEND E-MAIL INVITATION TO PATIENT'.

The Profile workspace also allows you set up a link to a patient's CareLink Personal account. Once the link is established, you can retrieve patient data stored on CareLink Personal anytime—without the need to have the patient present.

Before you begin

You may want to customize your patient profiles so they contain only the type of information you want to collect. To learn more, see [Patient profile preferences on page 12](#).

Also, a username and password is required when you set up the link to a patient's CareLink Personal account. The patient must be present to supply this data.

Adding new profiles

Each time you add a patient to the CareLink Pro system, you must start by filling out a profile for him or her.

- 1 Select **File > New Patient**, or click the **Add Patient** button. 

The **Profile** workspace is displayed.

NOTE: To add or change fields on the patient profile, click customize fields. See Patient profile preferences on page 12.

- 2 Fill in the fields in the **Patient Profile** section.
- 3 Click **SAVE**.

The new patient profile is added to the CareLink Pro database. A message is displayed that confirms the profile was saved.

Completing required fields

- 1 If a required field is not complete when you save a patient profile, a message is displayed next to that field. You will not be allowed to save the profile until you make an entry in the field.
- 2 Complete the field.
- 3 Click **SAVE**.
- 4 When the confirmation message displays, click **OK**.

Editing patient profiles

- 1 Make sure the patient's **Profile** workspace is open.
- 2 Click **EDIT**.
- 3 Edit the data in the **Patient Profile** section as needed.
- 4 Click **SAVE**.

A message is displayed that confirms the profile was saved.

Deleting patient data from the system

- 1 Make sure the patient's **Profile** workspace is open.
- 2 Verify that this is the patient you want to delete. Deleting a patient profile also removes all of his or her data from the CareLink Pro database and cannot be undone.
- 3 Click >> **delete patient record** above the synchronization section of the profile.
A message is displayed to alert you that all of the patient's data will be erased when you delete the record.
- 4 Click **Yes** to delete the patient's record.

Linking to CareLink Personal

If your patient permits it, you can set up a link to his or her CareLink Personal account. This Web-based tool allows patients to upload and store device-derived data and to run various therapy reports.

After you link to the patient's CareLink Personal account, you can retrieve the device data stored there. This is ideal for creating CareLink Pro therapy reports between office visits. It also reduces the need to read the patient's device in the office.

If patients do not yet have a CareLink Personal account, you can send them an e-mail inviting them to establish one.

Linking to an existing account

NOTE: The patient must be present to complete these steps.

- 1 Make sure your computer is connected to the Internet.
- 2 Open the patient's **Profile** workspace.
- 3 Make sure all required fields in the **Patient Profile** section are filled in.
- 4 Click **LINK TO EXISTING ACCOUNT**.

The CareLink Personal Log In screen is displayed.

- 5 Have the patient do the following:
 - a. Type in his or her Username and Password.
 - b. Click **Sign In**.

A **Grant Access** page is displayed, based on the patient's enrollment settings for language and region.

- 6 Have the patient do the following:
 - a. Read the **Terms of Use**.
 - b. Click to check the box next to **I agree to the Terms of Use above...**
 - c. Click **Grant Access**.
 - d. Let you know when the **Thank You** page is displayed.
- 7 If needed, print the Terms of Use for the patient by clicking the **Print** button. You are now linked to the patient's CareLink Personal account.

Sending an e-mail invitation

To send an e-mail inviting a patient to establish a CareLink Personal account, follow these steps:

- 1 Open the patient's **Profile** workspace.
- 2 Make sure all required fields in the **Patient Profile** section are filled in.

- 3 Click **SEND E-MAIL INVITATION TO PATIENT**.

E-Mail Invitation

Patient Name: SAMPLE PATIENT

E-Mail Address:

Language: English

Subject: Register to use Electronic CareLink Personal

Message:

Dear SAMPLE PATIENT:

You are receiving this message because your health care provider would like you to try Medtronic CareLink Personal - web-based therapy management software that will help you and your health care provider better manage your Diabetes. The software is designed to transform data from your MiniMed Paradigm insulin pump and a variety of glucose meters into useful information that will enable you and your doctor to make more informed treatment decisions.

To start using the system, follow the steps outlined below:

1. Visit <http://carelink.minimed.com>
2. Click on "Sign Up Now"
3. Complete the registration form

SEND **Cancel**

- 4 Make sure **Patient Name**, **E-mail Address**, and **Language** are filled in correctly.

- 5 Click **SEND**.

The patient's profile status area confirms the e-mail was sent.

Getting data from a linked account

If you are linked to a patient's CareLink Personal account, any new data from this account is automatically sent each time you open his or her patient profile in CareLink Pro.

NOTE: To ensure this happens, go to Tools > Options > General, and make sure there is a check next to "Synchronize with CareLink Personal."

Follow these steps to get a patient's CareLink Personal data any time after you have opened his or her patient profile:

- 1 Make sure the patient's **Profile** workspace is open, and that you are connected to the Internet.
- 2 Select **Tools > Synchronize Patient Data**.

The sync icon  on the patient's tab rotates. When the icon stops, the process is complete.

NOTE: If the patient no longer wants to share his or her CareLink Personal data, a message displays to let you know.

- 3 Any additional data retrieved from CareLink Personal will show up in the patient's reports.

Unlinking a patient's CareLink Personal account from CareLink Pro

You can unlink a patient's CareLink Personal account from CareLink Pro. This option is only available after a patient has been linked. It prevents CareLink Pro from continuing to retrieve data from the patient's CareLink Personal account. It does not affect the patient's personal usage of his or her CareLink Personal account.

- 1 Open the patient's record and access the **Profile** workspace.
- 2 Click **UNLINK ACCOUNT**.
- 3 Click Yes at the confirmation message. The patient's personal profile is no longer linked to CareLink Pro.

The status is changed to **Not linked**, and the **LINK TO EXISTING ACCOUNT** and **SEND E-MAIL INVITATION TO PATIENT** buttons are now displayed.

Hardware setup

To read data directly from a device, you must have the patient's device and any cables or communications devices required to transfer the data to your computer.

Alternatively, if patients have uploaded their device data to their CareLink Personal account, you can obtain the data by linking to their account. To link to a patient's CareLink Personal account, see [Linking to CareLink Personal on page 20](#).

Connecting devices


The diagrams that follow show communication setup between different devices. Review the diagrams to see how to connect devices to communicate with your computer.

Connection example for devices with a USB connector:


The following example shows the CareLink USB used as a communication device between the pump and the computer. For a list of supported communication devices, see [Supported devices on page 2](#).




Serial and USB cable connection examples:

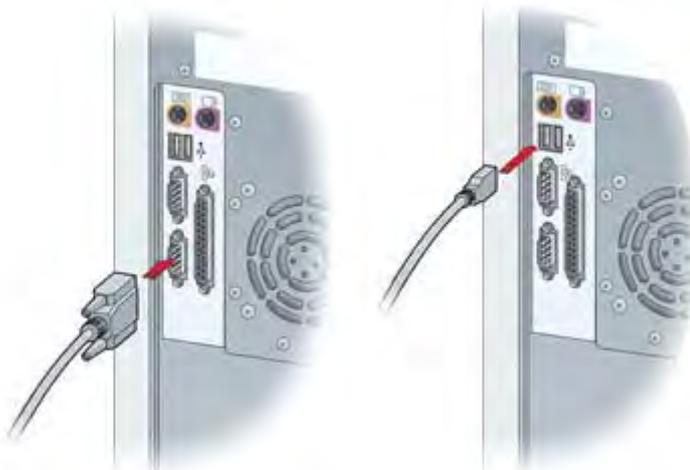

Optional ComLink for use with MiniMed Paradigm series pumps:

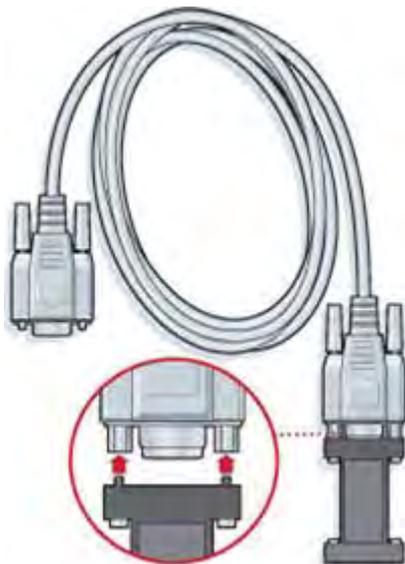


Optional Com-Station for use with the MiniMed 508 pump:

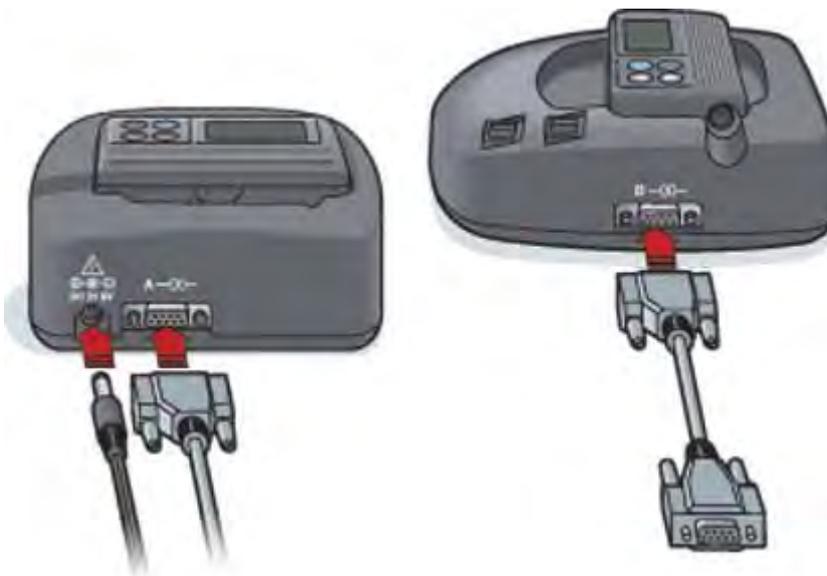

Devices workspace

Information that you will need to read a patient's device, such as the manufacturer, model, and serial number, is stored in the Devices workspace. Thus, you do not have to supply it each time you read data from the device.

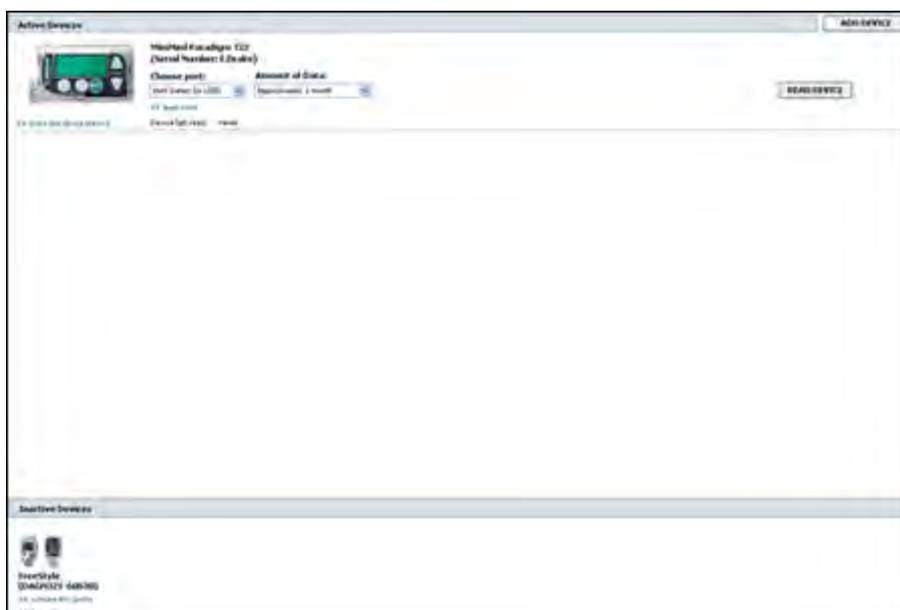

Devices on the Devices workspace are stored in one of two lists—Active Devices or Inactive Devices. When you add a device, it is automatically placed on the Active Devices list. You can only read data from devices displayed in the Active Devices list. These will likely be the devices your patient currently uses.

Other devices that belong to the patient, but are not currently used, can be stored in the Inactive Devices list. This keeps the information on file. These devices can be made active at any time.

Before you begin

Before you can open the Devices workspace for a patient, he or she must have a profile saved in the system. See [Adding new profiles on page 19](#).

To add a device or read data directly from it, the device must be communicating with the computer. See [Connecting devices on page 24](#) to learn how to set up devices to communicate with the computer. For a list of communication devices, see [Supported devices on page 2](#).

NOTE: To upload data from a patient's MiniMed 600 series pump, use either the black CareLink USB or a supported Bayer CONTOUR PLUS LINK 2.4 or Bayer CONTOUR NEXT LINK 2.4 meter that is not linked to the patient's pump. Using the patient's meter that is linked to the pump will cause a communication error.


Adding a device

You can get data from the patient's CareLink Personal account for a device not yet added. Such devices will automatically be added when data is synchronized between CareLink Personal and CareLink Pro.

NOTE: There can only be one active pump per patient. Adding a new pump will move the existing one to the inactive list.

Adding a Medtronic pump or Guardian monitor

- 1 Make sure the device you are adding is set up to communicate with the computer. (See [Connecting devices on page 24](#) for connection steps.)
- 2 Click the patient's tab or double-click his or her name on the Patient Lookup table.
- 3 Click **Devices**  to access the patient's Devices workspace.
- 4 Click **ADD DEVICE**.
- 5 Select **Medtronic Pump/Guardian**. The **Add Medtronic Pump/Guardian** Wizard is displayed.

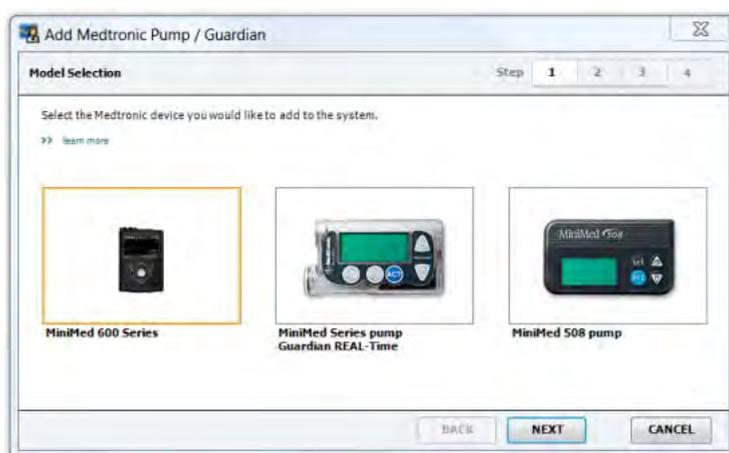

- 6 Click to select the pump or monitor model you are adding. The pump model is listed on the back of the pump or on the pump status screen.

If you select the **MiniMed 508 pump** option, go to Step 9.


- 7 Click **NEXT**. The **Serial Number** page is displayed.



- 8 Type the serial number in the **Device Serial Number** field. Use the examples in the image above to locate the serial number on the device you are adding, keeping in mind that the format of the serial number varies among devices. (If you need more help in locating it, click >>learn more.)

NOTE: An error message is displayed if you do not enter the correct serial number. Check the examples on this page, and verify that you are entering the correct number of characters from the back of the pump. If necessary, retype the characters.


- 9 Click **NEXT**. A **Communication Options** page similar to the following is displayed.

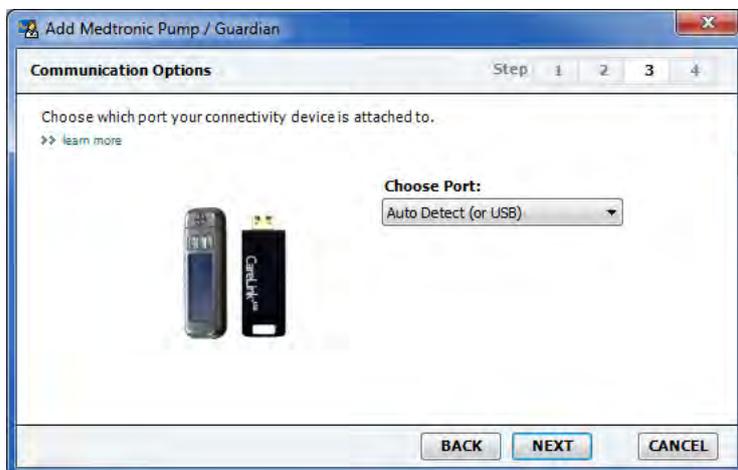

NOTE: If you are using a Bayer meter as a communication device, make sure that Bayer GLUCOFACTS™ DELUXE software is closed. Check the Windows system tray, shown below. If you see the GLUCOFACTS DELUXE icon, right-click the icon and select Exit.




- 10 Click **NEXT**. CareLink Pro auto detects the port to which your device is connected. The **Test Connection** page similar to the following is displayed.

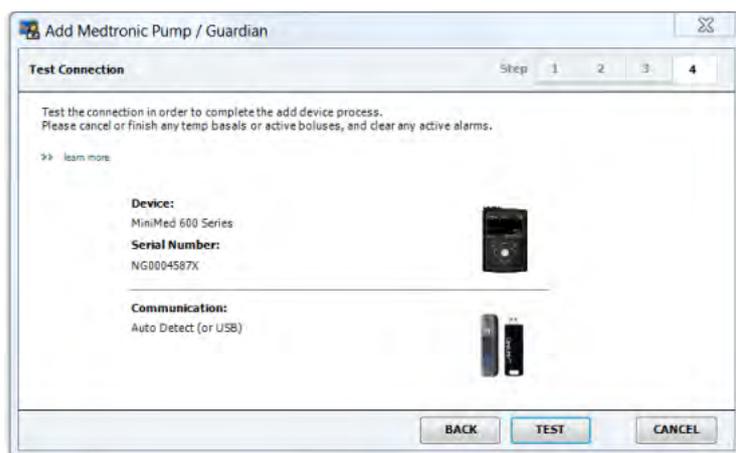

NOTE: This test does not read pump data, but verifies communication between the pump and the computer.

- 11 Click **TEST**. CareLink Pro attempts to connect to the selected pump or monitor. For the MiniMed 600 series pumps, a message in red is displayed on the **Test Connection** screen:

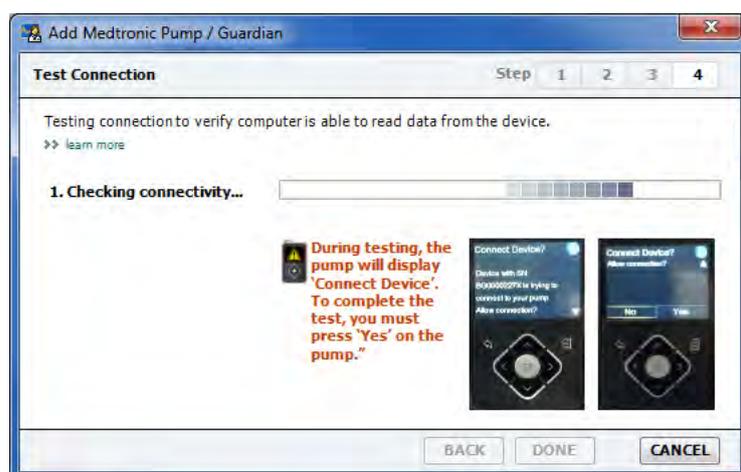

Follow the on-screen instructions.


After the connection test is complete, a message appears to let you know of the connection status between CareLink Pro and your device.

- 12 Do one of the following:
- If the test is successful, skip to step 13.
 - If the test fails, do the following and try again:
 - Verify that the communication device and the computer are connected properly.
 - Verify that the pump displays the home screen.
 - Click **BACK** at the bottom of each wizard page and verify that data is entered correctly.


13 Click **DONE**. The device is added to the patient's Active Devices list.

Adding a meter

- 1 Make sure the meter you are adding is in communication with the computer. (See [Connecting devices on page 24](#) for connection steps.)
- 2 Click the patient's tab or double-click his or her name on the Patient Lookup table.
- 3 Click **Devices**  to access the patient's Devices workspace.
- 4 Click **ADD DEVICE**.
- 5 Select **Blood Glucose Meter**. The **Add Blood Glucose Meter** Wizard is displayed.

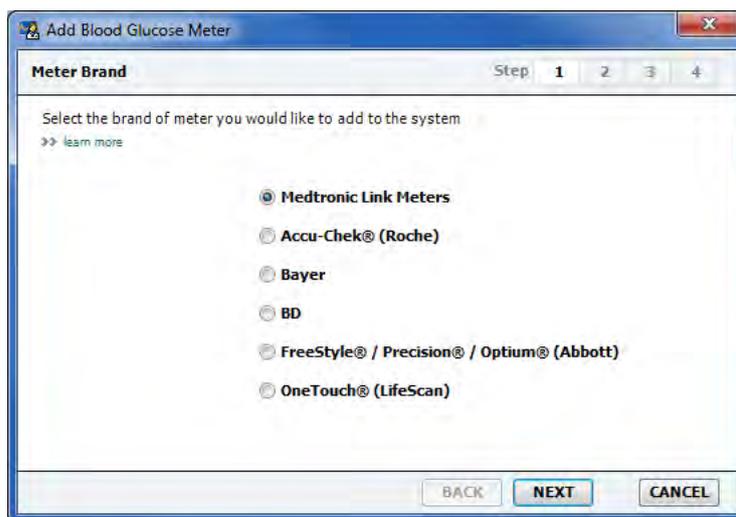

- 6 Click the option button to select the correct brand of meter.
- 7 Click **NEXT**. The **Meter Model** page is displayed (this page differs depending on the meter manufacturer).

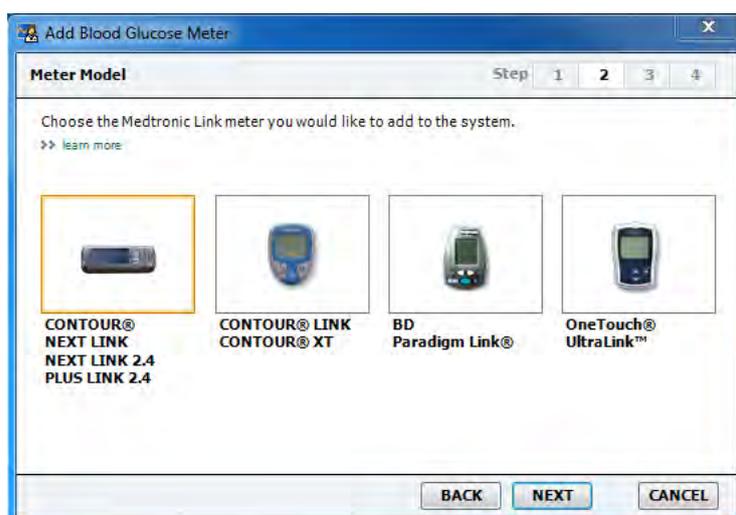

- 8 Click to select the meter model you are adding.

- 9 Click **NEXT**. The **Communication Options** page is displayed.



NOTE: Only those choices that are valid for the meter you are adding are available for selection.

- 10 Click **NEXT**. CareLink Pro auto detects the port to which the meter is connected on your computer. The **Test Connection** page similar to the following is displayed.



- 11 Click **TEST**. CareLink Pro attempts to link to the communication device.

If you are adding a supported Bayer meter with a USB connector, make sure that Bayer GLUCOFACETS™ DELUXE software is closed. Check the Windows system tray, shown here. If you see the GLUCOFACETS DELUXE icon, right-click the icon and select **Exit**.



A message displays to let you know if the connection was successful. If it was, go to the next step.

If not, make sure the hardware between the device and the computer is connected properly. Also, click **BACK** on the wizard to make sure the data you have entered is correct.

- 12 Click **DONE**. The meter is added to the patient's Active Devices list.

Making a device active or inactive

Patient devices can be moved between the Active Devices list and the Inactive Devices list as needed. A device must be active in order to read data from it.

You can have as many meters as you want on the Active Devices list, but only one pump. Make sure you want to inactivate the current active pump before you add a new one.

Inactivating a device

- 1 Click the patient's tab or double-click his or her name on the Patient Lookup table.
- 2 Click the **Devices** button to access the patient's Devices workspace. Devices may be listed under an equivalent device name. See [Supported devices on page 2](#).
- 3 Click >> **make this device inactive** under the device you want to make inactive. The device moves to the **Inactive Devices** list.

Re-activating a device

- 1 Click the patient's tab or double-click his or her name on the Patient Lookup table.
- 2 Click the **Devices** button. The patient's **Devices** workspace is displayed.
Devices may be listed under an equivalent device name. See [Supported devices on page 2](#).
- 3 Click >> **activate this device** under the device you want to make active.
The device moves to the **Active Devices** list.

Deleting a device

These steps will delete a device and its data from the Devices workspace and the CareLink Pro system:

- 1 Click the patient's tab or double-click his or her name on the Patient Lookup table.
- 2 Click the **Devices** button to access the patient's **Devices** workspace.
Devices may be listed under an equivalent device name. See [Supported devices on page 2](#).
- 3 Make sure the device is on the **Inactive Devices** list. If it is not, click >> **Inactivate this device** under its current listing.
- 4 Click >> **delete this device** under the device you want to delete. A message is displayed to alert you that the device and all of its data will be removed from the patient's record.
- 5 Click **YES** to delete the device.

The device and its data is removed from the **Devices** workspace and from the CareLink Pro system. Data from this device is no longer available for use in reports.

Reading device data

One way to get device data is to link to the patient's existing CareLink Personal account. (See [Linking to CareLink Personal on page 20.](#)) Another way is to read it directly from his or her device, as described here.

Data from your patient's device can be read by CareLink Pro if the device is on the Active Devices list and it is in communication with the computer. After you get this data, you can use it to create reports that help assess the patient's therapy management. See [About reports on page 41](#) for a brief description of the available reports.

CareLink Pro can gather the following data from an insulin pump:

- Various settings on the pump, such as the alert mode, the beep volume, and the time
- Basal insulin amounts delivered
- Bolus events and amounts delivered
- Bolus Wizard entries
- Priming amounts
- Suspend periods
- Sensor glucose readings over a period of time, on pumps with sensor capabilities

The system can also gather data from a Guardian REAL-Time system including:

- Sensor glucose (SG) readings
- Sensor coefficient values
- Sensor calibration factors
- Meal markers
- Insulin injections

Additionally, various information stored in a blood glucose meter can be uploaded to the system during a device read.

WARNING: Please cancel or finish any temp basals or active boluses, and clear any active alarms. The pump may be suspended for reading, depending on the pump model. Once the read is complete, please verify the pump has resumed if delivery was suspended.

CAUTION: Do not use the pump remote when the pump is being read. If the pump battery is low, the pump will not send data to the PC. Replace the battery if the status indicates battery power is low.

- 1 Click the patient's tab or double-click his or her name on the Patient Lookup table.
- 2 Make sure the patient's device is in communication with the computer. (See [Connecting devices on page 24.](#))
- 3 Click the **Devices** button to access the patient's **Devices** workspace.

Devices may be listed under an equivalent device name. See [Supported devices on page 2.](#)

- 4 Find the device you want to get data from on the **Active Devices** list, and make sure the **Choose port** data is correct.

For pumps, click the **Amount of Data** drop-down menu and select how much pump data you want CareLink Pro to read.

- 5 Click the associated **READ DEVICE** button.
- 6 Follow device-specific instructions, and click **OK**.
- 7 CareLink Pro displays a progress bar that updates to show how much of the device read has been completed.

If you click **CANCEL** as the device is being read, a message is displayed to alert you that cancelling the action may result in the loss of all of the data read so far. You will need to click the **READ DEVICE** button to restart the upload.

- To cancel, click **YES**.
- To continue reading device data, click **NO**.


When the system finishes reading data from the device, you will see a message that confirms the device read is complete.

- 8 Click **OK**.
 - For pumps, follow the instructions for taking them out of suspend mode.

If CareLink Pro is unable to get data from the device, see Troubleshooting for further guidance.

Reports workspace

CareLink Pro software provides a variety of reports to help you better manage your patients' diabetes treatment. The information contained in each report is based on data you obtain from a patient's devices and his or her CareLink Personal software account.

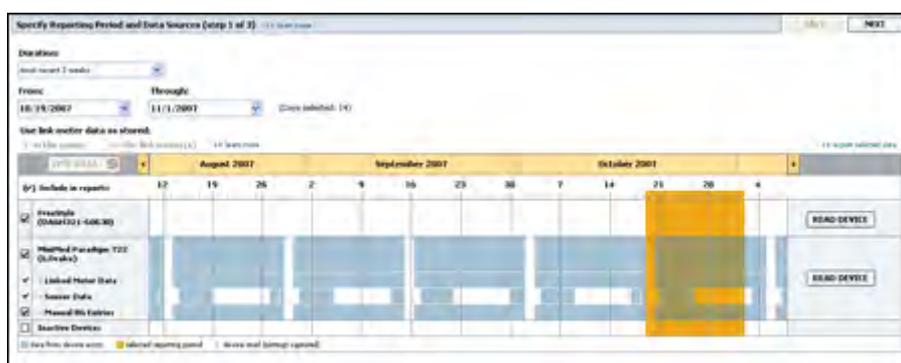

Reports can be generated on screen, sent directly to a printer, or saved as TIFF or PDF files that you can attach to an Electronic Medical Record (EMR). You can generate several report types through a single operation.

The data displayed through these reports is captured from the patient's devices, from his or her CareLink Personal account, or from both.

NOTE: More details about the report components, as well as sample reports are contained in the Report Reference Guide. You can access the Report Reference Guide through the CareLink Pro software by going to Help > View Report Reference Guide (PDF) and selecting the appropriate language.

Before you begin

If you have a period of time you want reflected in a report, you must have a patient's device data for that time period. You may also need to have the patient's device connected to the computer to get current data before running reports.

Be sure to take a close look at the **Verify Report Settings** step before running a report. This is where you can fine-tune a report to capture the patient data you want.

Creating reports

The following sections will help you better understand the reports that are available to you and the process you use to generate them.

If you are familiar with the reporting process and know what reports you would like to run, you can begin generating reports.

Opening the Reports workspace

Click the patient's tab or click the **Open Patient** button  and double-click the patient's name.

The **Reports** workspace is displayed.

NOTE: To make sure you have the latest device data from the patient's CareLink Personal account, click SYNC DATA.

Selecting the reporting period

- 1 To change how much time is reflected in the report(s), click the **Duration** drop-down menu and select the amount of time. (The maximum duration is 12 weeks.)
- 2 From and through dates are automatically set, unless you choose the **custom date range** option.


NOTE: If you select a date range longer than allowed, you get an error message. Adjust the duration or dates.

If you want a custom date range, click the **From** or **Through** drop-down menus and select the desired month, day, or year.

Data calendar

The data calendar area of the Reports workspace shows a three-month window of reporting information.

The blue bars represent device data. The orange bar represents the reporting period that you selected. Overlap in the device data and reporting period means you have data for some or all of the displayed reporting period.

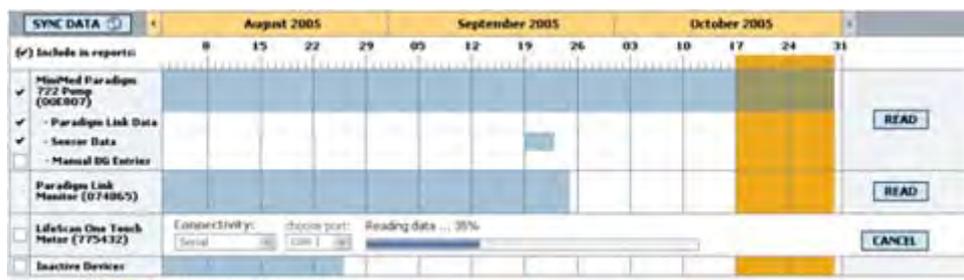

The data calendar area initially displays the most current three months. To see other months, click the arrow buttons   on either end of the months.

Selecting source data to include

- 1 If the patient uses a BG meter that links to his or her pump, click to choose one of the following options for reporting meter BG data:
 - *In the pump:* Advantages of this selection include that you only have to read data from the patient's pump, BG readings are time stamped by the pump, and the readings are tied directly to any Bolus Wizard calculations used. A disadvantage is that if there are communication difficulties between the pump and the linked meter, BG readings during that time may not get reported. Also, for MiniMed Paradigm pumps prior to the 522/722, any BG readings from Bolus Wizard calculations that are not acted on do not get reported.
 - *In the link meter(s):* The advantage of this selection is that all readings stored in the linked meter are reported. The disadvantage is that to correlate meter and pump data, you must have made sure that the pump and meter clocks were synchronized with one another. You must also read data from the pump and the linked meter separately.
- 2 To add device data to reports, select the check box next to the relevant device. You cannot add devices that were excluded due to your selection in step 1. To change this, select the other linked meter option.
- 3 To exclude device data from reports, clear the check box next to the relevant device. You cannot clear check marks related to the option you selected in step 1. To change these, select the other linked meter option.

Checking for device data

- 1 Look at the data calendar in the Reports workspace to see if the orange bar representing the reporting period overlaps with the blue bars representing device data.
- 2 If the bars overlap for the entire reporting period, you have data for your report(s). You can click **NEXT** and go to [Verifying report settings on page 39](#).
- 3 If the bars do not overlap or there is not enough overlap, you have a few choices:

- Adjust the reporting period.
- Get additional device data.

Getting additional device data

- 1 To get more data from a device, click the **READ DEVICE** button associated with the device.

The Read Device bar is displayed.



WARNING: Please cancel or finish any temp basals or active boluses, and clear any active alarms. The pump may be suspended for reading, depending on the pump model. Once the read is complete, please verify the pump has resumed if delivery was suspended.

CAUTION: Do not use the pump remote when the pump is being read. If the pump battery is low, the pump will not send data to the PC. Replace the battery if the device status screen indicates battery power is low.

- 2 Verify that the data in the **Choose port** field is correct for this device.
To change this setting, click the drop-down menu for the field and select a different setting.
- 3 Make sure the device is connected to your computer.
- 4 If the device is a pump, you can specify how much data to get from it. Click the **Amount of Data** drop-down menu and select an amount.

NOTE: If you select All available data, the system reads all data in the pump. This overwrites any existing duplicate data in the system.

- 5 Click **READ DEVICE**. Be sure to read the message that is displayed carefully because it provides specific instructions for reading the pump.
- 6 Follow the instructions and click **OK**.

The read device progress bar is displayed.

You can choose to cancel the read at any time by clicking **CANCEL**.

A message is displayed to confirm that the read is complete.

- 7 Click **OK**.
Device data is now visible within the data calendar.
- 8 Click **NEXT** at the top of the **Reports** workspace.

The Verify Report Settings step is displayed. This allows you to make sure the settings for this patient are correct before you run the report(s).

Verifying report settings

- 1 Make sure the **Glucose Target** settings are at the desired values. Type in these values, or click the up or down arrows in the **Low** and **High** fields to raise or lower the values. The target blood glucose settings you select will apply to the reports you generate. The reports will not show target ranges set on the pump or in CareLink Personal.

NOTE: Meter reading markers (||) are displayed on the wake-up and bedtime timeline, as well as on the meal markers timeline. Because some of the reports are based on data found within defined meal times, wake-up, or bedtime hours, it is important that a patient's Bolus Wizard event and meter reading markers are grouped appropriately.

- 2 To add a new meal period, click **ADD MEAL**. To edit an existing meal period, click anywhere within one of the meal periods along the timeline.

The Meal Period editor, located below the timeline, becomes active.

NOTE: You can have as many as five meal periods. The defaults are breakfast, lunch, and dinner.

- 3 Enter text or click arrows to select the settings you want.

If you only want to use these settings for this meal, clear the check box **Use these parameters for all of this patient's meals**.

- **Meal Name:** name you want to assign to the meal period.
- **Meal Time Period:** hours between which the meal occurs.
- **Pre-Meal BG Target (mmol/L or mg/dL):** low and high ends of the patient's before-meal glucose target range.
- **Pre-Meal Analysis Period:** time period that glucose will be analyzed prior to the start of a meal. The sensor glucose readings captured during this time are used in a detailed report analysis.
- **Post-Meal BG Target (mmol/L or mg/dL):** low and high ends of the patient's post-meal glucose target range.
- **Post-Meal Analysis Period:** time period that glucose will be analyzed after a meal. The sensor glucose readings captured during this time are used in a detailed report analysis.

You can change the length of an existing meal period or the wake-up and bedtime period by clicking on the start or end handles and dragging and dropping them along the timeline.

NOTE: Meal periods cannot overlap, but start and end lines can border one another. Meal periods must be at least 60 minutes in length.

- 4 To use the settings from this meal for all of the patient's other meals, make sure the check box next to **Use these parameters for all of this patient's meals** is selected.

- 5 After you finish creating or editing a meal period, click **SAVE**.
- 6 To remove a meal period, click **DELETE MEAL**. Click **DELETE** when asked to confirm.
- 7 CareLink Pro can remember these settings for this patient the next time you run a report for him or her. To save them for this patient, click **SAVE SETTINGS**.
- 8 Click **NEXT** at the top of the **Reports** workspace.

This is the Select and Generate Reports step of the process. It provides a list of report types as well as a Data Table that helps you choose to include or exclude certain days of data from the Daily Detail report(s).

Date	# of Meter Readings	Meter Readings Average (mg/dL)	Lowest Reading (mg/dL)	Highest Reading (mg/dL)	Total Insulin (U)	Bolus %	% of Correction Boluses	Sensor Average (mg/dL)
9/10/2010	7	163	77	350	39.90	58%	1	193 ± 72
9/11/2010	3	113	92	136	35.70	30%	—	—
9/12/2010	4	131	82	176	32.10	44%	—	—
9/13/2010	7	179	112	300	46.10	59%	—	—
9/14/2010	5	165	121	234	31.10	43%	—	—
9/15/2010	5	198	121	275	36.50	45%	1	—

NOTE: To modify the Data Table display, click >> customize columns. See Report Generation preferences on page 15.

- 9 To print the screen, click the **PRINT** icon .

Selecting report types and inclusion dates

- 1 Select the check box next to the report(s) you want to include in the report set.

NOTE: The Dashboard/Episode Summary report check box will not be available if there are less than five days of sensor data and pump data in the selected time period or if the data in the time period is from a Guardian monitor.

- 2 If data has been read from a pump or Guardian monitor more than once during this reporting period, there may be multiple device snapshots:
 - a. Make sure the check box is selected next to **Device Settings Snapshot**.
 - b. Click the drop-down arrow and select a snapshot date and time.
 - **Pump:** Select a snapshot from the patient's pump.
 - **Guardian:** Select a snapshot from the patient's Guardian monitor.

If either field is dimmed, there are no snapshots available during the reporting period.

- 3 Scroll through the Data Table to review the available Daily Detail report information.
 - You can sort the data in each column. Click the column heading to sort the data in ascending order. Click the heading again to sort the data in descending order.

NOTE: If there is no data for a certain date, that date cannot be selected.

- 4 Select the check box in the Data Table rows for any date for which you want a Daily Detail report.
 - To include or exclude all Daily Detail report dates with one click, select the check box at the top of the Data Table check box column.

Generating reports

- 1 After you verify your report selections, click **GENERATE REPORTS** at the top of the **Reports** workspace.

A list of options is displayed.
- 2 Select an option to preview, print, or save the report(s).

If you selected **Preview**, the **Preview** window is displayed.
- 3 Click the arrow buttons to navigate through multi-page reports.
- 4 Click one of the other buttons at the top of the **Preview** window to save or print the report(s).



- 5 To close this window, click the **Close** button  in the upper right corner of the window.

About reports

This topic provides a description of each report. More details about the report components, as well as sample reports are contained in the Report Reference Guide. You can access the Report Reference Guide through the CareLink Pro software:

- 1 **Help > View Report Reference Guide (PDF).**
- 2 Select a language for the Report Reference Guide.

The CareLink Pro reports share these common elements:

- **Report header** — The report header contains identifying information, such as the name of the report, the patient's name, and the source of the data.
- **Carbohydrates and blood glucose levels** — Within the graphs and charts, carbohydrate units are displayed in italics and blood glucose levels are displayed in bold.
- **Weekend data** — Weekend days are in bold so you can easily identify them.
- **Legends** — A legend of symbols appears at the bottom of each report. While a symbol may be used in multiple reports, the legends are unique to each report.

Dashboard and Episode Summary

The Dashboard and Episode Summary is a two-page report that is designed to provide a summary of a patient's overall glycemic control for a selected time period. The first page of the report is called the Therapy Management Dashboard, and the second page is the Episode Summary. A description of each page is provided below.

Therapy Management Dashboard

The Therapy Management Dashboard allows you to see the overall level of glycemic control by time of day. The Dashboard page plots sensor glucose overlay traces and insulin delivery information on a daily graph. The Dashboard also shows overnight time period and periods around mealtimes, to help you assess glycemic control before and after meals. Using these graphs, you can visually discern key clinical patterns such as hyperglycemia, hypoglycemia and variability within the overall graphical view of glycemic control. The Dashboard includes a statistical analysis of hypoglycemic and hyperglycemic patterns recurring at particular times of the day.

In addition, the Dashboard provides the ability to correlate glycemic control by time-of-day with key therapy modifiers, such as basal pattern, insulin absorption, insulin sensitivity, and carbohydrate ratios. This reduces the need to correlate events across multiple reports manually. Lastly, the Dashboard shows overall statistics of pump and sensor use.

Episode Summary

The upper section of the Episode Summary page provides details of sensor hypoglycemic and hyperglycemic episodes. It highlights the most critical episodes, and the frequency of correlated events of interest for further investigation. If applicable, the report enumerates the commonly known causes for hypoglycemic and hyperglycemic excursions and provides therapy considerations.

Note that the report may show sensor hypoglycemic or hyperglycemic episodes where there were no corresponding BG meter readings outside of the target range. Conversely, there may be BG meter readings outside of the target range where no sensor hypoglycemic or hyperglycemic episodes are reported.

At the bottom of the page, the Episode Summary provides overall observations regarding key behavioral or compliance measures related to insulin pump, CGM and BG meter usage. These observations may not be episode-related.

Adherence Report

The Adherence Report presents data that describes how insulin pumps and sensors are used and the patient's behavior relevant to his or her therapy. It answers the question, "Was there enough data to provide an accurate picture of how the patient uses his or her insulin pump and sensor, if applicable." It also answers the question, "Do patients adhere to the therapy as instructed?" It also indicates whether you may need to speak to your patients about the way they are managing their diabetes.

Sensor and Meter Overview Report

The Sensor and Meter Overview Report provides a graphical representation of the patient's daily sensor and meter-derived glucose levels and averages, including hourly breakdowns over 24 hours and as they relate to his or her meals and sleep patterns. Statistics on the patient's glucose readings and insulin usage are also included.

A similar analysis of sensor data is generated as the first page of this report if sensor data is available. When no sensor data is available, the meter data analysis page will be generated as the first page.

The final page(s) of the report shows the day-to-day level and quality of your patient's glycemic, carbohydrate, and insulin control. Each page shows how that control varies during each day across the entire reporting period up to a 14 day maximum per page.

Logbook Report

The Logbook Report provides meter glucose, carbohydrate, and insulin data for each day in the reporting period. It provides a diary of events recorded hourly, as well as daily averages and totals. Each page contains up to 14 days. If the reporting period exceeds 14 days, extra pages are generated.

Device Settings Snapshot

The Device Settings Snapshot Report presents a snapshot of the settings for the patient's pump or Guardian REAL-Time monitor for a specific date and time. This can help you understand other reports or can simply document your patient's settings.

The pump or monitor settings are recorded only when the device is read. If the device was not read during the reporting period, no settings will be available.

Daily Detail Report

The Daily Detail Report shows glucose data, carb amounts, and the patient's insulin usage for the selected day. A separate report is generated for each day you select from the Data Table.

The Daily Detail Report provides a detailed look at each day you select. If you see a significant reading or trend in a patient's summary and overview reports, you can use the Daily Detail Report to the details to see an hour-by-hour record of insulin delivered and glucose levels recorded.

Exporting data

You can export device data that is acquired and stored by CareLink Pro. This gives you all of a patient's device data to use for statistics or the creation of specialized reports or charts. The .csv file can be imported into Microsoft® Excel® or certain clinical statistics programs where you can further manipulate the data.

The .csv file contains data recording the actions of the device. For example, it lists the recording of meter readings, the pump receiving the meter reading value, or change in basal rate.

NOTE: This is an advanced feature and requires you to be familiar with the raw device data. It also requires proficiency with any software into which you import the .csv file.

Follow these steps to use the CareLink Pro export feature:

- 1 Click the patient's tab or click the **Open Patient** button  and double click the patient's name.

- 2 Make sure the **Reports** workspace is displayed.
- 3 Use the **Duration** or **From/Through** fields to set the dates and length of the report.
The maximum duration you can select is 12 weeks.
- 4 Click the **export selected data** link.
The **Export Data to CSV File** dialog box is displayed.
- 5 Navigate to the location where you want to store the .csv file on your computer. If you want to change the name of the file, type it into the **File name** box.
- 6 Click **SAVE**.

NOTE: For more information about the data displayed in CSV files, see the CSV data appendix.

The .csv file is now saved on your computer in the location you selected. You can now choose to import it into any program that supports this file type.

System administration

It is important that you regularly back up the CareLink Pro database. The database stores all system data that has accumulated in your patients' records, including profile information, device-derived data, and report settings.

It is also important that you have the latest version of CareLink Pro. Updated versions are available periodically and may contain significant enhancements.

Applying software updates

You will receive software updates on a CD. Download the update to your computer by following the instructions in the CareLink Pro Installation Guide.

NOTE: *The database should be backed up before a software update is applied. See [Backing up the database](#) on page 45.*

Backing up and restoring the database

It is a good idea to establish a regular schedule by which to perform database backups. This will help ensure that it is done regularly and will minimize the risk of data loss.

If you are backing up or restoring the database, the system displays an alert message if there are active users of the software on other computers.

Backing up the database

The following steps let you back up the current database to the location you select.

- 1 Make sure all patient records are closed.
- 2 Select **Tools > Backup Database**.

NOTE: *Database backups can be saved on a network drive or to removable storage (such as a DVD, CD, or USB drive).*

- 3 Navigate to the location on your computer where you want to save the backup file. If you want to change the name of the backup file, type it into the **File name** box.
- 4 Click **Save**. A progress bar is displayed while the database is saved.
A message is displayed when the backup is complete.
- 5 Click **OK** to close the message.

Restoring the database

The current database may need to be replaced if it can no longer be accessed or used. The more current your backup, the less data you will lose if you replace the database.

CAUTION: When you restore the database with a backup copy, you lose all the new data created in the current database since the selected backup copy was made.

The following steps let you select a backup copy to replace the current database.

- 1 Make sure all patient records are closed.
- 2 Select **Tools > Restore Database**.
- 3 Select the backup file you want to use to replace the current database (usually the most recent).
- 4 Click **Open**. A warning message is displayed to remind you about the data that may be lost if you continue the database restore.
- 5 To continue, click **OK**. A progress bar is displayed while the database is being restored.
A message is displayed when the database is restored.
- 6 Click **OK** to close the message.

When the system is unavailable

If you attempt to start the system while another user is performing a backup or restore, you will receive a message notifying you that the system is not available. You will not be able to access the system until the task is complete.

Do one of the following:

- Wait for the process to complete and for the system to become available.
- Click **CANCEL** to exit and try again later.

Troubleshooting

This topic is designed to help you solve issues that may occur while using CareLink Pro software. It also contains instructions for uninstalling the CareLink Pro software if necessary.

Not connected to the database

An error message stating that you are not connected to the database indicates one of the following:

- The database has been moved. The database must be located in the same place that was selected during installation of the CareLink Pro software. If it has been moved, it must be moved back to the location selected during installation.
- You are not connected to the network drive where the database is located. If the database is located on a network drive, the network may occasionally experience problems that prevent you from accessing the drive. Contact your computer support department for help in reconnecting to the network drive where the database is located.

Forgot the clinic password for CareLink Pro

If no one can remember the password your clinic uses to log in to CareLink Pro, the CareLink Pro software must be reinstalled and a new database created. After you reinstall the software, you will not be able to access any patient information that was in the previous database. Store the password that you created during the new installation somewhere in the office so that you will not lose future data.

Device read errors

The table below describes only a selection of device errors that need further clarification.

Error	Explanation
<p>The selected serial port could not be opened. Another operation might be in progress on that port. Please wait until the port is available, or select another port.</p>	<p>Please verify that the com port selected is not in use by another program, or select a different port. Try rebooting the computer you are using and then try the device read again. The hardware (such as the cable) connected to the port or the port itself may be bad. Connect the hardware to another port and try the device read again to help determine the problem.</p>
<p>Auto Detect could not find the device on any available port. Please check the cable connection, device battery & status and try again, or try specifying a serial port.</p>	<p>The system did not find the device you are trying to add. Do the following:</p> <ul style="list-style-type: none"> • Verify that the cable is connected to the computer. • Verify that the device battery is charged. • Rather than selecting Auto Detect, try specifying the PC serial port to which the cable is connected.
<p>The system was unable to communicate with pump serial (<serial #>). Ensure the communication device is inserted, the pump is on the home screen, press 'yes' when the pump asks to 'Allow connection'.</p>	<p>The system could not establish communication with the pump. Do the following:</p> <ul style="list-style-type: none"> • Verify that the communication device is properly inserted. • Make sure the pump displays the home screen when you start the procedure. • When prompted, on the pump, scroll down to the bottom of the Connect Device screen and select Yes.
<p>Device not found at selected serial port. Please check the cable connection, device battery & status and try again, try selecting a different port, or try to Auto Detect the device.</p>	<p>Check the connection between the cable and the PC, and verify that the device battery status is fine. If so, try either selecting a different PC serial port number, or choose the Auto Detect option.</p>
<p>Unable to communicate with the device. Please ensure you've attached and selected the correct device, check the cable connection, device battery and status, and try again.</p>	<p>Verify all settings selected for the device read, including device name, serial number, and type of connection. Also check to make sure that the device, cable, and PC are connected properly. Verify the battery and alarm status of the device are okay. Try the read again.</p>
<p>Retrying (n%)</p>	<p>The system could not read a value and will retry communication for up to 50 times. Do one of the following:</p> <ul style="list-style-type: none"> • Wait for the system to retry communication. • Cancel and restart the procedure.
<p>The link device was found, but the device (<serial #>) is not responding. Please verify the device's serial number, place device closer to link device to minimize interference, check device battery and status.</p>	<p>The system has found the device, but it is not responding. Do the following:</p> <ul style="list-style-type: none"> • Verify that the correct serial number is entered. • Move the pump or monitor closer to the communication device. • Move the pump or monitor away from possible source of radio frequency interference, such as cell phones, cordless phones, or other devices. • Verify that the device battery is charged. • Verify the pump delivery status.
<p>This pump is delivering a temp basal. Please cancel the temp basal or wait until it is finished, and then try again.</p>	<p>Your pump is delivering a Temp basal. Do one of the following and then try uploading from the pump again:</p> <ul style="list-style-type: none"> • Wait until the Temp basal delivery is finished. • Cancel the Temp basal delivery.
<p>This device has active errors or alarms. Please clear the alarms and try again.</p>	<p>There are active alarms on the pump that prevent it from being read. Read the alarm instructions for clearing the alarm. Clear the alarm and try the pump read again.</p>

Error	Explanation
This pump is delivering a bolus. Please cancel the bolus or wait until it is finished, and then try again.	Your pump is delivering a bolus. Do one of the following and then try uploading from the pump again: <ul style="list-style-type: none"> • Wait until the bolus delivery is finished. • Cancel the bolus delivery.
The device returned invalid entries; all data read will be discarded.	Contact your local country representative (see Assistance on page 2).
More than one CONTOUR NEXT LINK / CONTOUR NEXT LINK 2.4 / CONTOUR PLUS LINK 2.4 devices were found connected to this computer. Please connect only the device that is associated with this patient.	When uploading a Bayer link meter, verify that only one patient's meter is connected to the computer.
The system was unable to communicate with pump serial (<serial #>). Please ensure that one of the supported link devices is connected.	Verify that a supported communication device, such as a black CareLink USB or a supported Bayer link meter, is connected to the computer and that the device is properly connected to the USB port.
The system was unable to communicate with pump serial (<serial #>). Please ensure that the link meter is NOT connected with the pump.	Make sure you are not using the patient's link meter as a communication device. If you are, switch to a different communication device, such as the black CareLink USB or a supported Bayer meter that the patient has not linked with his pump.
The system was unable to communicate with pump. The pump is busy. Please wait for the current operation on the pump to complete before retrying.	The system could not communicate with the pump. Verify that there is no active Bolus or Temp Basal on the pump. If necessary, wait until the current operation is finished before attempting another upload from the pump.
The system was unable to communicate with pump serial (<serial #>). Ensure the communication device is inserted, the pump is on the home screen, press 'yes' when the pump asks to 'Allow connection'.	The system could not communicate with the pump. Verify the following conditions are met: <ul style="list-style-type: none"> • The pump is in range, close to the communication device. • The communication device is connected to the computer. • The pump displays the home screen. • The serial number is entered correctly. • Alarms are cleared on the pump. • No active Bolus or Temp Basal deliveries are in progress. • When prompted, on the pump, scroll down to the bottom of the Connect Device screen and select Yes.

Report creation errors

Multiple data entries for the same date

If multiple data entries exist for the same date and time for the same device, the system considers this to be a conflict that it cannot resolve. Reports created using this device data will omit the portion of data that overlaps.

You can try to adjust the reporting period to miss the overlapping data. Or, you can remove the device from the system and then add it back again to clear the previous readings.

System is going to ignore data

If the time on a device has been changed causing overlaps or gaps in data of three hours or longer, the system does not include that portion of data when creating reports.

Backup and restore errors

The database cannot be locked

This means that you are using the system in a multi-user environment, and other users are logged in. The system will not allow a database backup to be performed while other users are potentially performing tasks that may affect the database. Once all other users exit CareLink Pro, you can perform the database backup.

A database backup or restore is not completing

Other users cannot log in and the backup or restore cannot complete. Please contact your local country representative (see [Assistance on page 2](#)).

A restore database fails

The database backup file you are attempting to use in the restore process is corrupt. Try restoring with a different backup file.

Uninstalling the software

If you need to uninstall CareLink Pro, complete the following steps:

- 1 Open the Windows Control Panel. If needed, refer to the Microsoft documentation for instructions on how to access the Control Panel on your operating system.
- 2 Select the option to **Uninstall a program** or **Add or Remove Programs**.
- 3 In the window that opens, scroll down to **Medtronic CareLink Pro** and click on it.
- 4 Click **Remove** or **Uninstall**. The Install Shield Wizard is displayed.
- 5 Click **Next**. A message is displayed asking you to confirm that you want to remove the application.
- 6 Click **Yes**. The uninstall program runs and removes the program and all of its files from your computer. When it is done, a message displays on the wizard screen confirming the uninstall.
- 7 Click **Finish**.

Icon table

The icons and symbols on the packaging labels and the equipment are described in the following table:

Description	Icon
One per container/package	(1X)
CD enclosed	
Consult instructions for use	
Date of manufacture (Year)	
Catalogue number	REF
Conformité Européene (European Conformity). This symbol means that the device fully complies with MDD 93/42/EEC.	
Lot number	LOT

CSV data

When you export report data from the CareLink Pro software, it is exported into a .csv file. This file can then be imported into a spreadsheet application, such as Microsoft Excel. See the CSV file column definitions for a complete listing of the data that can be contained in a CSV file.

The CSV file contains the name and Patient ID for the patient, the reporting period, and identifies each device included in the report.

Column data definitions

Column heading	Definition
Index	The order in which data was recorded in the device.
Date	The date data was recorded in the device.
Time	The time data was recorded in the device.
New Device Time	The new date and time if this was changed in the device.
BG Reading (mmol/L or mg/dL)	The blood glucose reading recorded by the meter, Guardian, or pump. If the data is from a pump or Guardian, this column reflects manual BGs and BGs received from a Link meter.
Linked BG Meter ID	The serial number for the meter that sent a particular blood glucose reading to the device.
Basal Rate (U/h)	The active basal insulin delivery rate in units per hour.
Temp Basal Amount	If a temp basal was applied on the pump, this value is the temp basal amount.
Temp Basal Type	The type of temporary basal adjustment (insulin rate or percent of basal).
Temp Basal Duration (m)	The length of time in minutes for the temporary basal insulin delivery (see type above).
Bolus Type	The bolus insulin delivery type [Normal, Square, Dual (normal part), or Dual (square part)].
Bolus Volume Selected (U)	The number of units of insulin selected to be delivered during the bolus insulin delivery.

Column heading	Definition
Bolus Volume Delivered (U)	The number of insulin units actually delivered during the bolus insulin delivery.
Programmed Bolus Duration (h)	Duration of a square bolus or the square portion of a Dual Wave™ bolus.
Prime Type	Manual or fixed. Manual is used just after a rewind, to fill the infusion set tubing with insulin before inserting it. Fixed is used after infusion set insertion to fill the soft cannula with insulin after removing the introducer needle.
Prime Volume Delivered (U)	The number of units of insulin actually delivered for the prime.
Alarm	The name of the alarm that occurred.
Suspend	Identifies the suspended state of the pump.
Rewind	Date and time the device was rewound.
BWZ Estimate (U)	The bolus insulin estimate calculated by the Bolus Wizard feature.
BWZ Target High BG (mmol/L or mg/dL)	The setting for the high end of the blood glucose target range, used by the Bolus Wizard feature.
BWZ Target Low BG (mmol/L or mg/dL)	The setting for the low end of the the blood glucose target range, used by the Bolus Wizard feature.
BWZ Carb Ratio	The setting for insulin-to-carbohydrate ratio. If grams are used as the units, the ratio is the number of grams covered by one unit of insulin. If exchanges are used for units, the ratio is the number of insulin units used to cover one exchange.
BWZ Insulin Sensitivity	The setting for insulin sensitivity. Insulin sensitivity is the amount the blood glucose level is reduced by one unit of insulin. This is used by the Bolus Wizard feature.
BWZ Carb Input	Amount of carbohydrates entered into the Bolus Wizard and used to estimate a bolus.
BWZ BG Input (mmol/L or mg/dL)	Blood glucose reading when entered into the Bolus Wizard and used to estimate a bolus.
BWZ Correction Estimate (U)	Units of bolus insulin to give for blood glucose level correction, as calculated by the Bolus Wizard feature.
BWZ Food Estimate (U)	The estimated units of bolus insulin to give to cover the expected amount of carbohydrate consumption, as calculated through the Bolus Wizard feature.
BWZ Active Insulin (U)	The amount of active insulin calculated to be left in the body from prior bolus insulin deliveries when determining the estimated bolus amount through the Bolus Wizard feature.
Sensor Calibration BG (mmol/L or mg/dL)	The BG value used for calibrating the sensor in mmol/L or mg/dL.
Sensor Glucose (mmol/L or mg/dL)	The sensor glucose value.
ISIG value	Input signals (ISIG), being read from the sensor, measured in nanoamperes (nA).

Column heading	Definition
Event Marker	<p>A record of the following events entered by the user including:</p> <ul style="list-style-type: none"> • Insulin amount • Carb amount • Carb amounts (others) • Exercise • Start of the day • End of the day
Suspend Column	<p>Displays one of the suspend states:</p> <ul style="list-style-type: none"> • ALARM_SUSPEND • USER_SUSPEND • AUTO SUSPEND • LOWSG-SUSPEND • NOTSEATED_SUSPEND • SMARTGUARD_PREDICTED_LOW_SG • NORMAL_PUMPING

More about CSV files exported by CareLink Pro

The title at the top of the CSV file includes the following:

- patient's name
- a list of selected devices and their serial numbers
- selected date range

Each block of columns has a title that includes the following:

- name of the device to which the block of data applies
- serial number of that device

If data is not displaying as expected

A number of different factors can cause the CSV data to display differently than expected.

- Date or time changes on the device can change the sequence or cause records outside the selected date range to be shown.
- If there is a large gap between device reads, data for that device may be displayed in multiple blocks.

Glossary

A1C - Glycosylated hemoglobin

A1C Test - Hemoglobin A1C test, used to interpret blood glucose level over a period of time.

Area Under the Curve (AUC) - Indicates the amount in high and low excursions as determined by preset values. It complements the excursion data. Excursion data indicates the frequency of highs and lows. AUC indicates the magnitude of events by showing how far out of the target range they are and how long they last.

Audio bolus - The pump can be programmed so the user hears a beep when he or she selects a bolus insulin amount (0.5 or 1.0 units) to be delivered. This is useful for situations when it is difficult to see the buttons on the pump.

Authenticate - A means by which a user verifies their identity by use of a username and password combination when entering a Web site area that contains sensitive patient information or data.

Basal insulin - An amount of insulin delivered automatically by an insulin pump based on preprogrammed profiles and personalized rates set in the pump. The pump delivers a daily pattern of insulin that typically covers "background" insulin needs during periods of fasting (i.e., overnight and between meals).

Basal patterns - Users can program up to three different basal rate patterns into their pump for the delivery of basal insulin: Standard, A, and B. For each pattern, there is the option of setting up to 48 basal rates.

Basal profile - A basal rate with a start and stop time. Users can program several different profiles into their pump, each with a different basal rate, during a 24-hour period of time to achieve better glucose control.

Basal rate - The pump setting that provides a continuous infusion of insulin to keep the blood glucose stable between meals and during the night. Basal insulin mimics pancreatic insulin delivery—which meets all the body's non-food related insulin needs.

BG - Blood Glucose

Bolus insulin - A dose of insulin given to cover an expected rise in blood glucose (such as the rise after a meal) or to lower a high blood glucose down to target range.

Cal Reminder - The pump will trigger a Meter BG By HH:MM alert automatically every 12 hours, signaling that the current calibration value is no longer valid. The value of the Cal Reminder is the amount of time before the current calibration value expires by which the user wants to be reminded to calibrate. For example, if the Cal Reminder is set to 2 hours, the Meter BG By HH:MM alert will occur 2 hours before calibration is required.

Carb ratio (carbohydrate ratio) - Used when counting carbohydrates in grams. The amount of carbohydrates covered by one unit of insulin. (Also see exch ratio.)

Carb units - The food entry when using the Bolus Wizard feature. Entered as (carbohydrate) grams or exchanges.

CareLink™ Personal - A therapy management Web application that allows uploading, logging and reporting of diabetes data via the Internet.

CH - Carbohydrate

ComLink - A radio frequency (RF) transceiver device used to download MiniMed series insulin pump or Guardian REAL-Time Monitor data to the computer.

Com-Station - A device used to download MiniMed 508 pump and pass-through third-party meter data to the computer.

Correction bolus - The amount of insulin needed to return a high blood glucose level back down to target range.

Correction bolus factor - How much 1.0 unit of insulin will lower your blood glucose. This factor is used to calculate a correction bolus amount when your blood sugar is high. $(BG \text{ level}) - (BG \text{ target}) = X$. $X \div (\text{correction bolus factor}) = \text{correction bolus amount}$

CSV (Comma Separated Values) file - A common text file format that contains comma-delimited values. It can be compiled using any spreadsheet software to generate a database for statistical analysis.

Dual Wave™ bolus - Combination of a Normal bolus that is delivered immediately, then followed by a Square Wave bolus. The Square Wave portion is delivered evenly over a period of time.

Easy Bolus™ - A feature that lets you deliver a Normal Bolus in preset increments using only audio or vibrate confirmation.

Exch ratio (exchange ratio) - Used when counting carbohydrates as exchanges. The amount of insulin required to cover one (1) carbohydrate exchange. (Also see carb ratio.)

Express bolus - Method of delivery for any bolus type using the express bolus button on the pump.

Food bolus - A dose of insulin given to cover the expected rise in blood glucose that occurs after eating.

HbA1c - Glycosylated hemoglobin

HbA1c Test - Hemoglobin A1C test, used to interpret blood glucose control or average of levels over a 2- to 3-month period of time.

High Glucose - The pump will alarm if the sensor indicates that the user's sensor glucose is at or above this value. You have the option to turn this feature on or off.

Hyperglycemic - Elevated blood glucose as seen by monitoring blood glucose levels with or without any or all of the following symptoms: nausea, vomiting, blurred vision, headache, gastric distress, frequent urination of large amounts, and lethargy.

Hypoglycemic - Low blood glucose as seen by monitoring blood glucose levels, with or without any or all of the following symptoms: excessive hunger, shaking or tremors, perspiration, dancing visions, light-headedness, headache, blurred speech, sudden mood swings, or personality change.

Infusion set - The apparatus used for inserting and securing a cannula below the skin and transporting insulin to the insertion site via tubing from the pump.

Insulin concentration - The strength or type of insulin the doctor has prescribed for the user. This affects the rate of insulin the pump delivers. If the user's insulin concentration changes, the basal patterns and the maximum basal and bolus rates must be reprogrammed in the pump.

Insulin sensitivity - The amount of mmol/L (or mg/dL) that your blood glucose (BG) level is reduced by one unit of insulin. (Bolus Wizard data.)

ISIG - Sensor values that indicate whether the transmitter electronics in a sensor-augmented system are working properly. If you see an ISIG value that is less than 24.00 nA or more than 29.00 nA, call for product assistance. It may be time to replace your transmitter.

Ketone test - Ketone is a waste product that is produced when the body is forced to burn body fat instead of glucose for energy. It may be a sign of lack of insulin in the body. The Ketone test measures the amount of ketone concentrated in the blood or urine.

Link

- (1) A connection a patient can set up between his meter and pump so they can communicate wirelessly with each other, available only on some devices.
- (2) A connection a healthcare provider can set up with a patient's CareLink Personal account.

Low Glucose - The pump will alarm if the sensor indicates that the user's sensor glucose is at or below this value. You have the option to turn this feature on or off.

Low Glucose Suspend - This feature is set up to stop insulin delivery when your sensor glucose reaches or drops below your Low Suspend limit.

Low reservoir warning - Programmable warning that notifies you with an alert when either a specified number of units remain in the reservoir of your pump, or a specified amount of time remains before the reservoir will be empty.

Manual bolus - Optional item available in the BOLUS MENU when the Bolus Wizard is active. One method of programming a bolus without the Bolus Wizard.

Max basal insulin - The maximum amount of basal insulin that the pump will deliver at one time. (Set by the user.)

Max bolus - The maximum amount of bolus insulin that the pump will deliver at one time. (Set by the user.)

Mean Absolute Difference % (MAD%) - Represents the level of accuracy in calibration of the sensor to BG meter readings. The lower this number, the greater the calibration accuracy. MAD % is calculated by taking the difference between closely occurring pairs of sensor glucose and BG meter readings, dividing by the BG meter reading, and then averaging across all pairs.

Meter - A medical device for determining the approximate concentration of glucose in the blood. A small drop of blood is placed on a disposable test strip, which the meter reads and uses to calculate the blood glucose level. The meter then displays the level in mmol/L or mg/dL.

Meter option - Feature that allows the pump to receive BG readings from a linked BG meter.

Normal bolus - An immediate delivery of a specified unit amount of insulin.

Pattern feature - Extended pump feature that allows you to program optional basals (Pattern A, Pattern B) that support activities or glucose patterns that are not a part of your day-to-day routine, but are usual in your lifestyle. Such activities could be a sport that you do once a week, a change in your sleep pattern over the weekend, or hormonal changes during a menstrual cycle.

Pattern, standard - Your normal basal that supports your usual day-to-day activity. When the Patterns feature is off, the pump uses your standard (basal) pattern.

RF - Radio frequency (RF).

SmartGuard™ - A feature that can automatically stop and resume insulin delivery based on your sensor glucose values and low limit.

Square Wave™ bolus - Bolus delivered evenly over a specified time period (30 minutes to 8 hours).

Square Wave portion - (Sq) The second part of a Dual Wave bolus. The Square Wave portion delivers evenly over a period of time after the NOW portion delivers.

Step - Measurement of insulin that you set and use for Easy Bolus delivery.

Suspend - Function on the pump that stops all insulin delivery. Any current bolus and/or prime deliveries are canceled. The basal delivery is paused until restarted.

Suspend before low - A feature that suspends insulin delivery when the sensor predicts sensor glucose value is approaching your low limit.

Suspend on low - A feature that suspends insulin delivery when your sensor glucose value reaches or falls below your low limit.

Temp - Temporary.

Temp basal (tmp basal) - Temporary, one-time basal insulin with a specified amount and duration. Used to support insulin needs for special activities or conditions that are not part of the normal daily routine.

Transmtr ID - The serial number of the transmitter currently in use.

Upload - The process for transferring pump or meter data to the CareLink Personal server.

User - The registered person.

µL - micro liter

Index

A

- about reports 41
 - Adherence report 42
 - Daily Detail report 43
 - Dashboard and Episode Summary 41
 - Device Settings Snapshot 43
 - Logbook report 43
 - Sensor & Meter Overview report 42
- activating devices 32
- adding a device to the system 27
- adding a Guardian monitor to the system 27
- adding a meter to the system 30
 - equivalent meter names to choose 4
- adding a patient 19
- adding a patient's device to the system
 - Guardian monitor 27
 - meters 30
 - pumps 27
- adding a pump to the system 27
- Adherence report
 - about 42

B

- backing up the database 45
- basic CareLink Pro tasks 7
- buttons on the toolbar 8

C

- cables for connecting devices to computer
 - serial 24
 - USB 24
- CareLink Personal
 - getting data 21
 - linking to an account 20
 - email invitation 20
 - existing account 20
- checking
 - for device data for reports 37
- closing patient profiles 10

- ComLink 3, 25
- communication devices supported by CareLink Pro 3
- communications devices supported 2
- Com-Station 3
- connecting devices to computer 24
 - cables 24
 - computer connections 24
 - serial 24
 - USB 24
 - meter options 24
 - optional components 25
 - ComLink 25
- connecting devices to your computer
 - computer connections 24
 - serial 24
 - USB 24
- contraindications 5
- copying the database for backup 45
- creating patient profiles 19
- creating reports 36
 - checking for device data 37
 - getting new device data 38
 - making your own report 43
 - opening the reports workspace 36
 - previewing 41
 - printing 41
 - saving 41
 - selecting devices 37
 - selecting report types and inclusion dates 40
 - selecting the reporting period 36
 - verifying report settings 39
- CSV files
 - exporting device data to 43

D

- Daily Detail report
 - about 43
- Dashboard and Episode Summary
 - about 41
- data communications cable 3
- data communications cable supported 4

- database
 - copying for backup 45
 - restoring with backup copy 46
- deleting a patient's device from the system 32
- device data
 - getting data from CareLink Personal 21
 - getting it from a patient's device 33
 - linking to CareLink Personal 20
 - email invitation 20
 - existing account 20
- Device Settings Snapshot
 - about 43
- devices
 - activating 32
 - adding to the system 27, 30
 - Guardian monitor 27
 - meters 30
 - pumps 27
 - checking for data for reports 37
 - connecting to computer 24, 25
 - computer connections, serial 24
 - optional components, ComLink 25
 - connecting to your computer 24
 - computer connections, serial 24
 - deleting 32
 - deleting from the system 32
 - exporting data 43
 - getting data 33, 38
 - new data for reports 38
 - inactivating 32
 - ordering 4
 - selecting for reports 37
 - storing in the system 32
 - inactivating 32
 - making active 32
 - supported 2, 3, 4
 - ComLink 3
 - Com-Station 3
 - glucose meters 2
 - insulin pumps 2
 - meter data communications cable 3, 4
 - supported by CareLink Pro 2
- devices workspace
 - adding devices 27, 30
 - Guardian monitor 27
 - meters 30
 - pumps 27
 - deleting devices 32
 - getting device data 33
 - storing devices 32
 - inactivating 32
 - making active 32
- downloading software updates 45

E

- editing patient profiles 19
- email invitation to set up a CareLink
 - Personal account 20
- equivalent devices
 - alternative meter names to choose 4

- existing CareLink Personal account
 - linking to 20
- exporting device data 43

F

- features of CareLink Pro 1
 - security 2

G

- general preferences
 - setting 11
- generating reports 41
 - previewing 41
 - printing 41
 - saving 41
- getting a patient's device data 33
- getting device data
 - from CareLink Personal 21
 - linking to CareLink Personal 20
 - email invitation 20
 - existing account 20
 - new data for reports 38
- global system preferences
 - setting 11, 12, 13, 14, 15, 17
 - general preferences 11
 - open patient preferences, choosing data 14
 - patient lookup preferences 14
 - patient lookup preferences, changing column order 14
 - patient profile preferences 12
 - patient profile preferences, adding a custom field 13
 - patient profile preferences, changing field order 13
 - patient profile preferences, choosing data fields 13
 - report generation preferences, changing column order 17
 - report generation preferences, choosing data 15
 - understanding 11
- glucose meters supported 2
- glucose meters supported by CareLink Pro 2
 - Guardian monitor
 - adding to the system 27
 - Guardian monitors
 - inactivating 32
- Guide Me feature 9

H

- hardware connections 24
 - cables 24
 - computer connections 24
 - serial 24
 - USB 24

- meter options 24
- optional components 25
 - ComLink 25
 - USB 24
- HelpLine, contacting 2
- how to use this user guide 4

I

- icons 51
- inactivating devices 32
- inclusion dates
 - selecting for reports 40
- indications for use 5
- insulin pumps supported 2
- insulin pumps supported by CareLink Pro 2

K

- key features of CareLink Pro 1

L

- linking to CareLink Personal accounts 20
 - email invitation 20
 - existing account 20
 - getting data 21
- Logbook report
 - about 43
- logging in
 - to CareLink Pro 8

M

- Medtronic MiniMed products
 - ordering 4
- meter cable 3
- meter data communications cable
 - supported 3, 4
- meter name
 - equivalent devices 4
- meters
 - activating 32
 - adding to the system 30
 - connecting to computer 24, 25
 - computer connections, serial 24
 - computer connections, USB 24
 - optional components, ComLink 25
 - connecting to your computer 24
 - computer connections, serial 24
 - computer connections, USB 24
 - deleting 32
 - getting data 33
 - inactivating 32
 - options for communicating with
 - computer 24
 - ordering 4
 - supported 2

N

- navigating
 - workspaces 8
- navigating the CareLink Pro GUI 8
- navigation bar
 - workspaces 8
- notification of software updates 45

O

- online device data
 - getting the data 21
 - linking to CareLink Personal 20
 - email invitation 20
 - existing account 20
- open patient preferences
 - setting 14
 - choosing data 14
- opening
 - reports workspace 36
- opening CareLink Pro 8
 - entering your password 8
 - logging in 8
- opening patient profiles 10
- optional devices for communicating with
 - computer 25
- ordering
 - devices 4
 - Medtronic MiniMed products 4
 - meters 4
 - pumps 4
- overview of CareLink Pro 1

P

- password
 - entering for CareLink Pro 8
- patient lookup preferences
 - setting 14
 - changing column order 14
- patient profile preferences
 - setting 12, 13
 - adding a custom field 13
 - changing field order 13
 - choosing data fields 13
- patient profiles
 - closing 10
 - creating 19
 - editing 19
 - opening 10
- PC
 - connecting devices 24
 - computer connections, serial 24
 - computer connections, USB 24
 - connecting devices to it 24, 25
 - computer connections, serial 24
 - computer connections, USB 24
 - optional components, ComLink 25

- preferences
 - system 11, 12, 13, 14, 15, 17
 - setting 11
 - setting, general preferences 11
 - setting, open patient preferences, choosing data 14
 - setting, patient lookup preferences 14
 - setting, patient lookup preferences, changing column order 14
 - setting, patient profile preferences 12
 - setting, patient profile preferences, adding a custom field 13
 - setting, patient profile preferences, changing field order 13
 - setting, patient profile preferences, choosing data fields 13
 - setting, report generation preferences 15
 - setting, report generation preferences, changing column order 17
 - setting, report generation preferences, choosing data 15
 - understanding 11
- previewing
 - reports 41
- primary CareLink Pro tasks 7
- printing
 - reports 41
- product
 - overview 1
- profiles
 - closing 10
 - creating 19
 - editing 19
 - opening 10
- pumps
 - activating 32
 - adding to the system 27
 - communicating with the computer 33, 38
 - guidelines 33, 38
 - connecting to computer 24, 25
 - computer connections, serial 24
 - computer connections, USB 24
 - optional components, ComLink 25
 - connecting to your computer 24
 - computer connections, serial 24
 - computer connections, USB 24
 - deleting 32
 - getting data 33
 - inactivating 32
 - ordering 4
 - supported 2

R

- report generation preferences
 - setting 15, 17
 - changing column order 17
 - choosing data 15

- report settings
 - verifying 39
- report types
 - selecting for reports 40
- reporting period
 - selecting 36
- reports
 - about 41, 42, 43
 - Adherence report 42
 - Daily Detail report 43
 - Dashboard and Episode Summary 41
 - Device Settings Snapshot 43
 - Logbook report 43
 - Sensor & Meter Overview report 42
 - creating 36, 37, 38, 39, 40, 41
 - checking for device data 37
 - getting new device data 38
 - opening the reports workspace 36
 - previewing 41
 - printing 41
 - saving 41
 - selecting devices 37
 - selecting report types and inclusion dates 40
 - selecting the reporting period 36
 - verifying settings 39
 - creating your own 43
 - previewing 41
 - printing 41
 - saving 41
 - understanding 41
- reports screen
 - overview 35
- restoring the database 46

S

- safety 5
- saving
 - reports 41
- security features of CareLink Pro 2
- selecting
 - devices for reports 37
 - report types and inclusion dates 40
 - the reporting period 36
- Sensor & Meter Overview report
 - about 42
- serial connections 24
- settings
 - verifying for reports 39
- software updates 45
- starting the software 8
 - entering your password 8
 - logging in 8
- storing a patient's device on the system 32
 - inactivating 32
 - making active 32
- supported communications devices 2
- supported devices 2
 - ComLink 3
 - communication devices 3

- Com-Station 3
- glucose meters 2, 4
 - equivalent devices 4
- insulin pumps 2
- meter communications cable 3
- supported meters 2
- supported pumps 2
- symbols 51
- system preferences
 - setting 11, 12, 13, 14, 15, 17
 - general preferences 11
 - open patient preferences, choosing data 14
 - patient lookup preferences 14
 - patient lookup preferences, changing column order 14
 - patient profile preferences 12
 - patient profile preferences, adding a custom field 13
 - patient profile preferences, changing field order 13
 - patient profile preferences, choosing data fields 13
 - report generation preferences 15
 - report generation preferences, changing column order 17
 - report generation preferences, choosing data 15
- understanding 11

T

- toolbar for CareLink Pro
 - buttons 8
- troubleshooting 47

U

- understanding reports 41
 - Adherence report 42
 - Daily Detail report 43
 - Dashboard and Episode Summary 41
 - Device Settings Snapshot 43
 - Logbook report 43
 - Sensor & Meter Overview report 42
- updating software 45
- USB connections 24
- user guide
 - conventions 4
- user interface
 - Guide Me 9
 - navigating 8
 - toolbar 8
- user safety
 - contraindications 5
 - indications for use 5
 - warnings 5

V

- verifying report settings 39

W

- warnings 5
- workspaces 8